
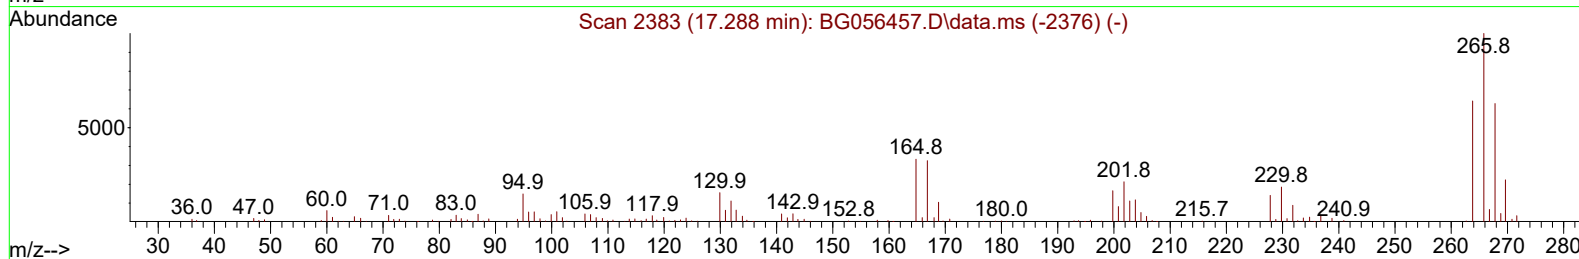
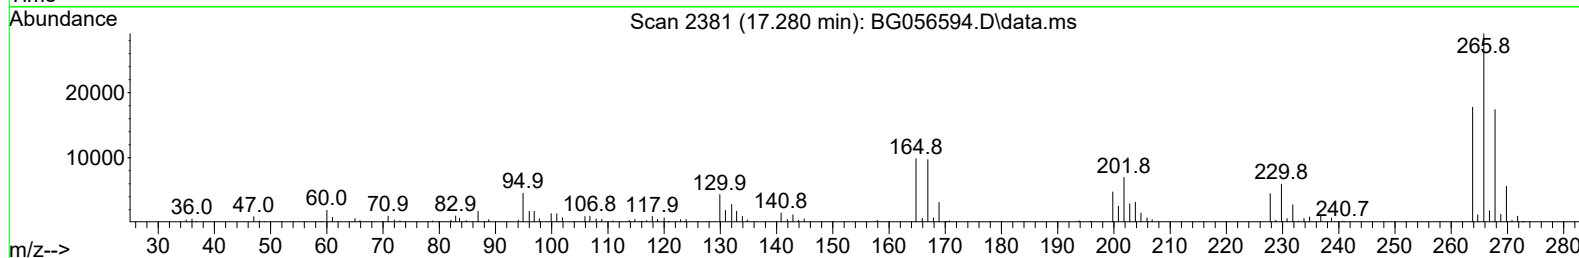


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020923\
Data File : BG056594.D
Acq On : 9 Feb 2023 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 02:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

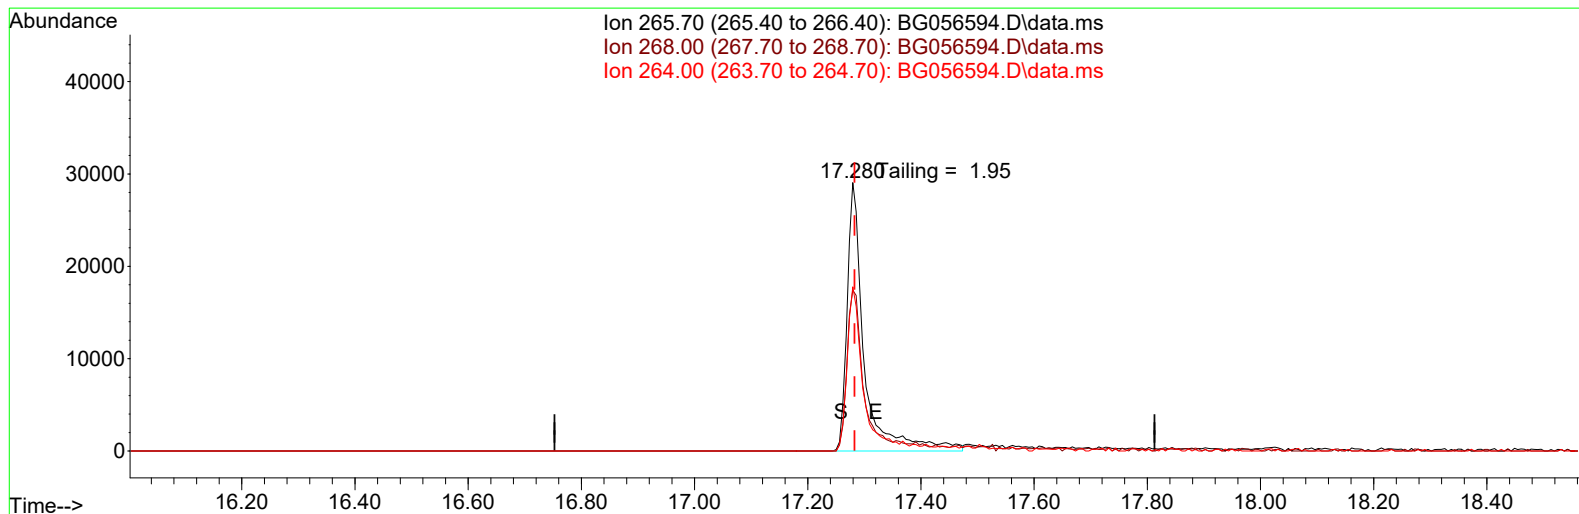

TIC: BG056594.D\data.ms

(70) Pentachlorophenol (C)




17.280min (-0.003) 18901.86 ng

response 59656

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	59.90
264.00	64.20	65.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020923\
Data File : BG056594.D
Acq On : 9 Feb 2023 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 02:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

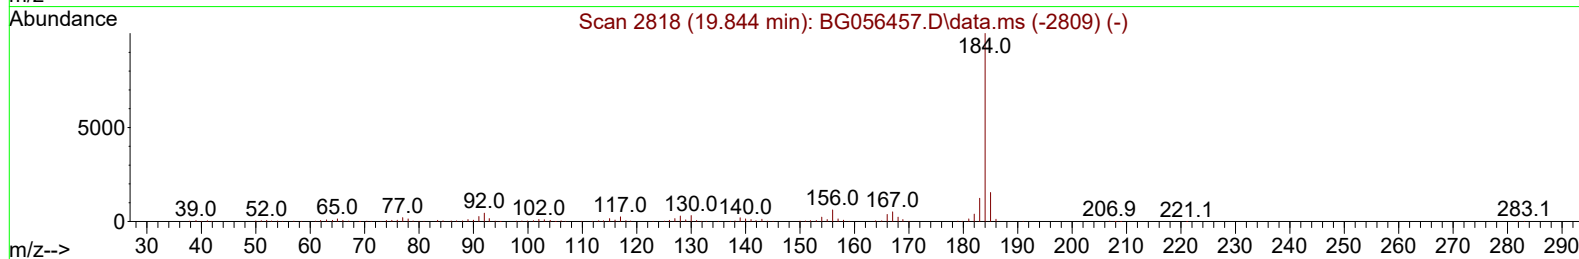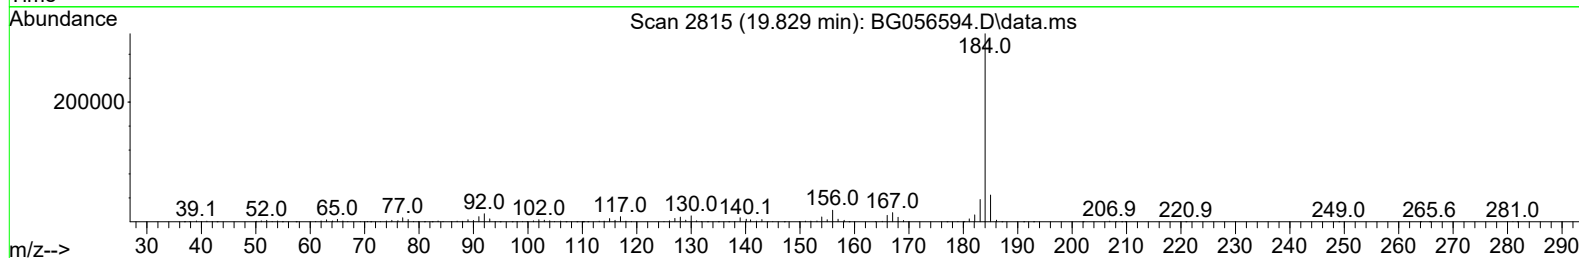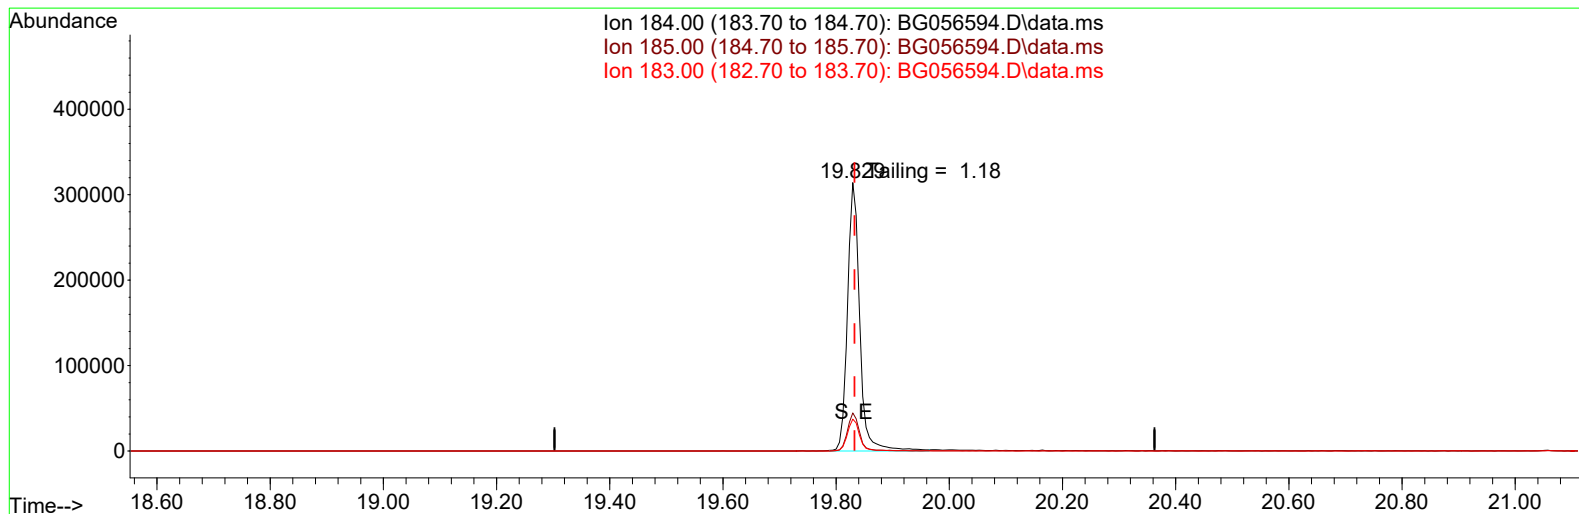

TIC: BG056594.D\data.ms

(77) Benzidine**19.829min (-0.003) 296482.92 ng****response 473368**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.23
183.00	12.30	11.86
0.00	0.00	0.00