


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020923\  
Data File : BG056594.D  
Acq On : 9 Feb 2023 10:54  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Feb 08 03:02:11 2023

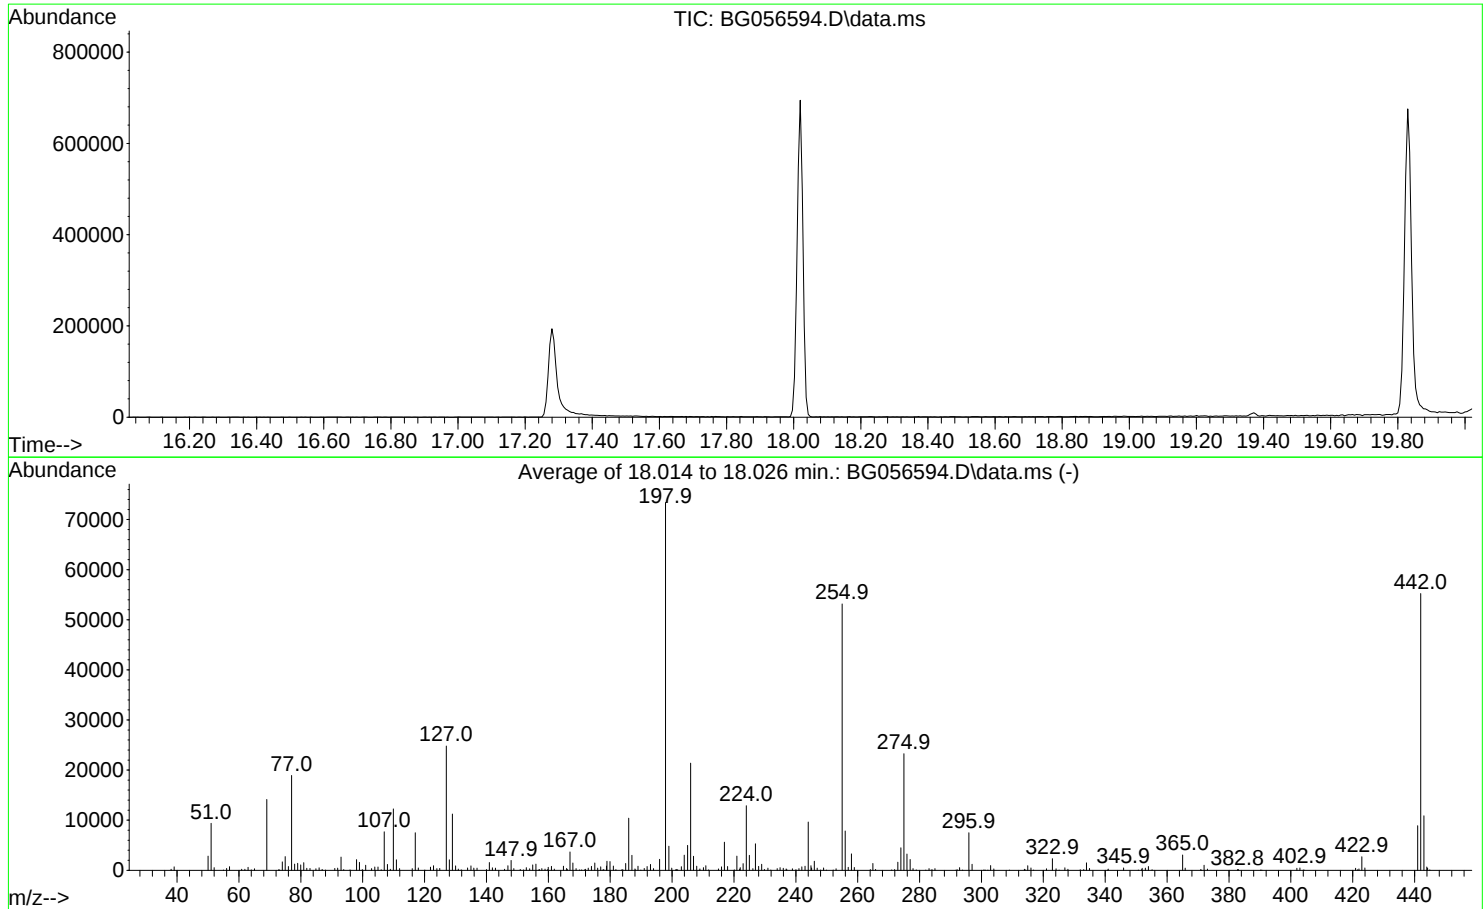




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 12.8         | 9370       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 19.3         | 14138      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 33.8         | 24805      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 73419      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 4804       | PASS                |
| 275            | 198             | 10              | 60              | 31.7         | 23264      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 3043       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.1         | 8894       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 55221      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 10885      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020923\  
 Data File : BG056594.D  
 Acq On : 9 Feb 2023 10:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 10 02:27:18 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Feb 08 03:02:11 2023  
 Response via : Initial Calibration

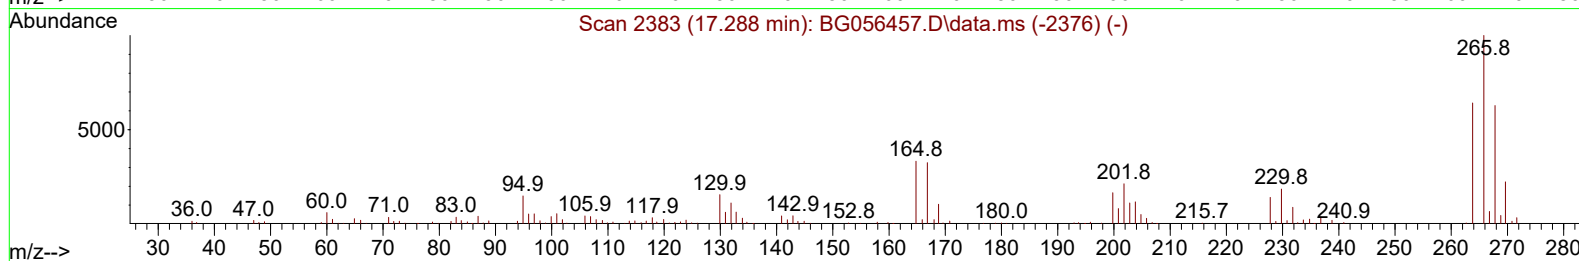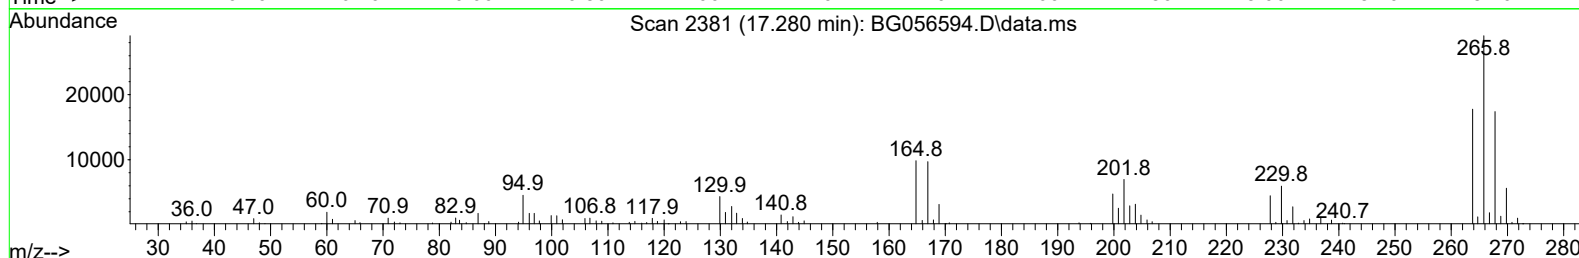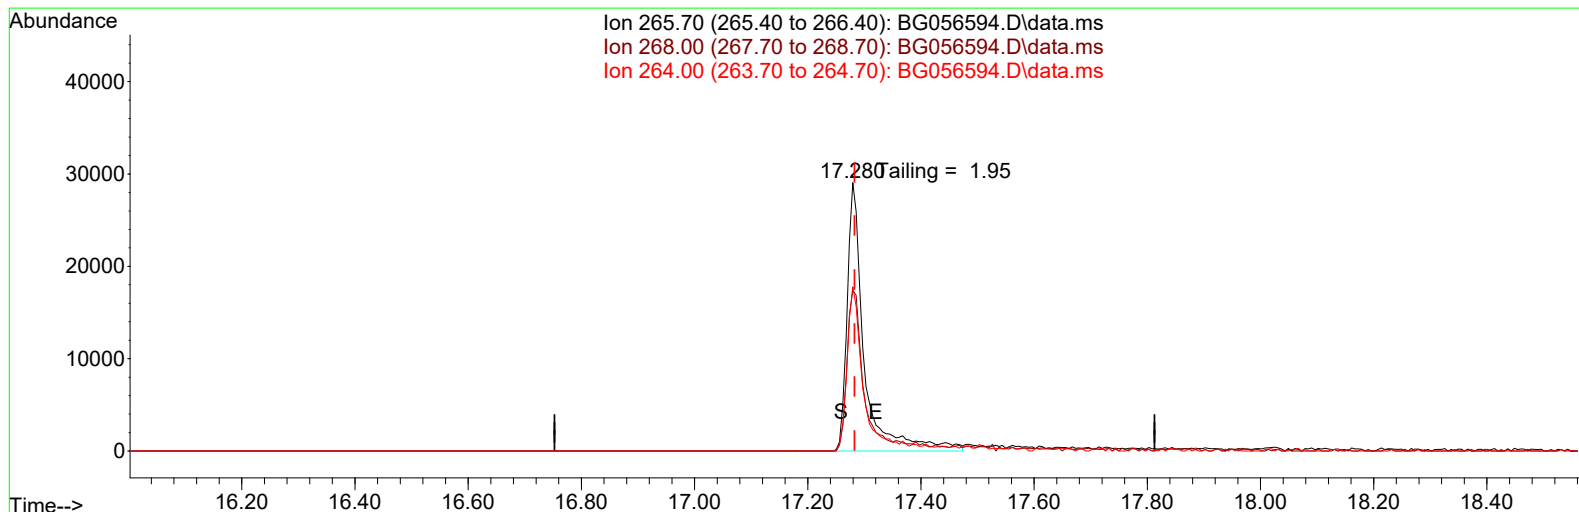

TIC: BG056594.D\data.ms

**(70) Pentachlorophenol (C)**

17.280min (-0.003) 18901.86 ng




response 59656

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.80  | 59.90  |
| 264.00 | 64.20  | 65.35  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020923\  
Data File : BG056594.D  
Acq On : 9 Feb 2023 10:54  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Feb 10 02:27:18 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Feb 08 03:02:11 2023  
Response via : Initial Calibration

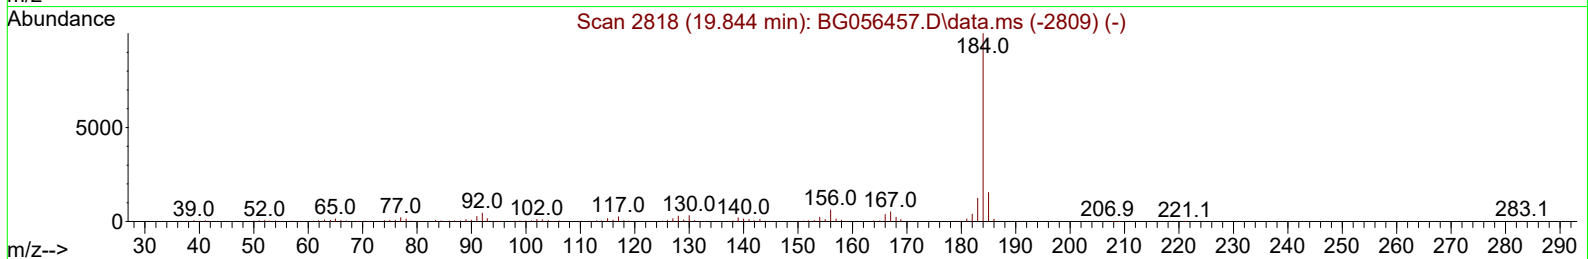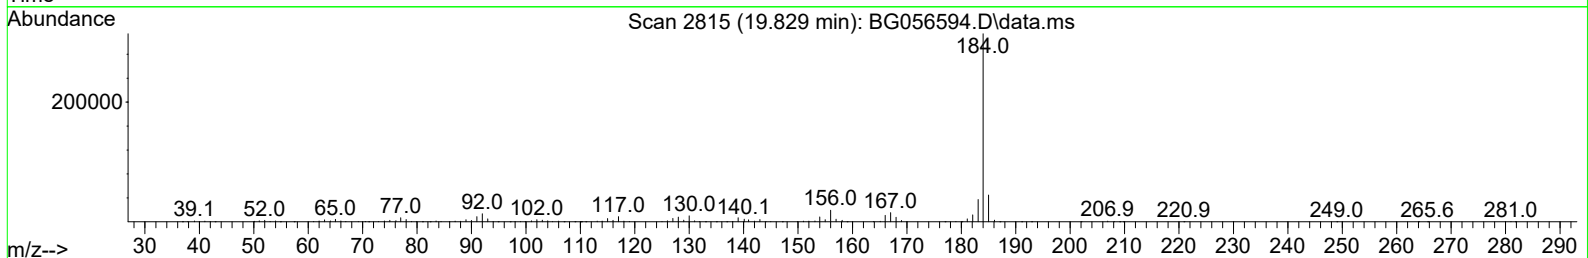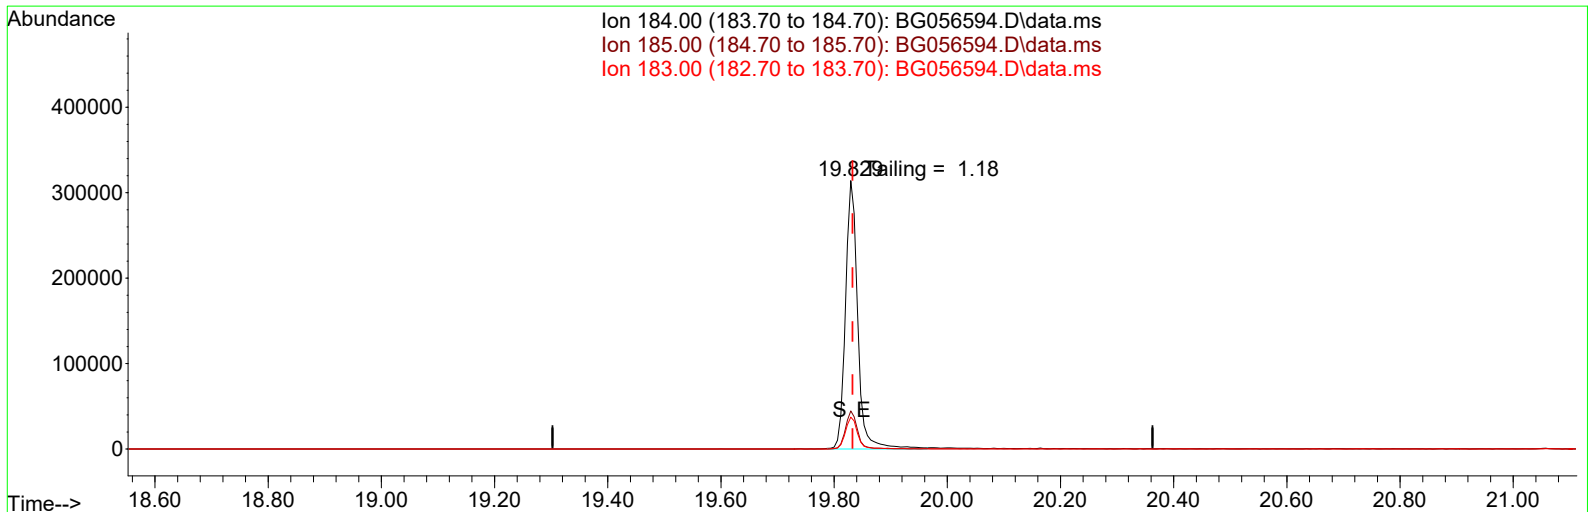

TIC: BG056594.D\data.ms

**(77) Benzidine**

**19.829min (-0.003) 296482.92 ng**

**response 473368**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.40  | 14.23  |
| 183.00 | 12.30  | 11.86  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/9/2023      | BNA_G            | BG056594.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 245861           | 21.057             |
| DDD           | 6936             | 20.611             |
| DDE           | 774              | 20.106             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7710          | 253571           | 3.04               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP