

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
 Data File : BG020843.D
 Acq On : 10 Feb 2016 16:42
 Operator : SJ/UM
 Sample : H1390-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04Q1

Quant Time: Feb 11 04:07:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 11 04:03:47 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	21859	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	110209	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	64344	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	129776	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	120181	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	111382	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.61	96	2347	5.21	ng/uL	0.00
5) Phenol-d5	7.41	99	61921	27.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	33755	28.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	50679	29.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	54982	28.56	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	27173	30.73	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	28426	32.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	50604	29.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.23	131	80360	35.65	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	171908	31.05	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	219926	32.52	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	30585	27.59	ng/ul	0.00
58) Fluorene-d10	15.87	176	149779	31.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	15592	24.79	ng/ul	0.00
71) Anthracene-d10	17.72	188	216624	33.78	ng/ul	0.00
79) Pyrene-d10	19.99	212	217200	35.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	208328	33.75	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.33	163	73603	12.77	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
Data File : BG020843.D
Acq On : 10 Feb 2016 16:42
Operator : SJ/UM
Sample : H1390-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04Q1

Quant Time: Feb 11 04:07:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 11 04:03:47 2016
Response via : Initial Calibration

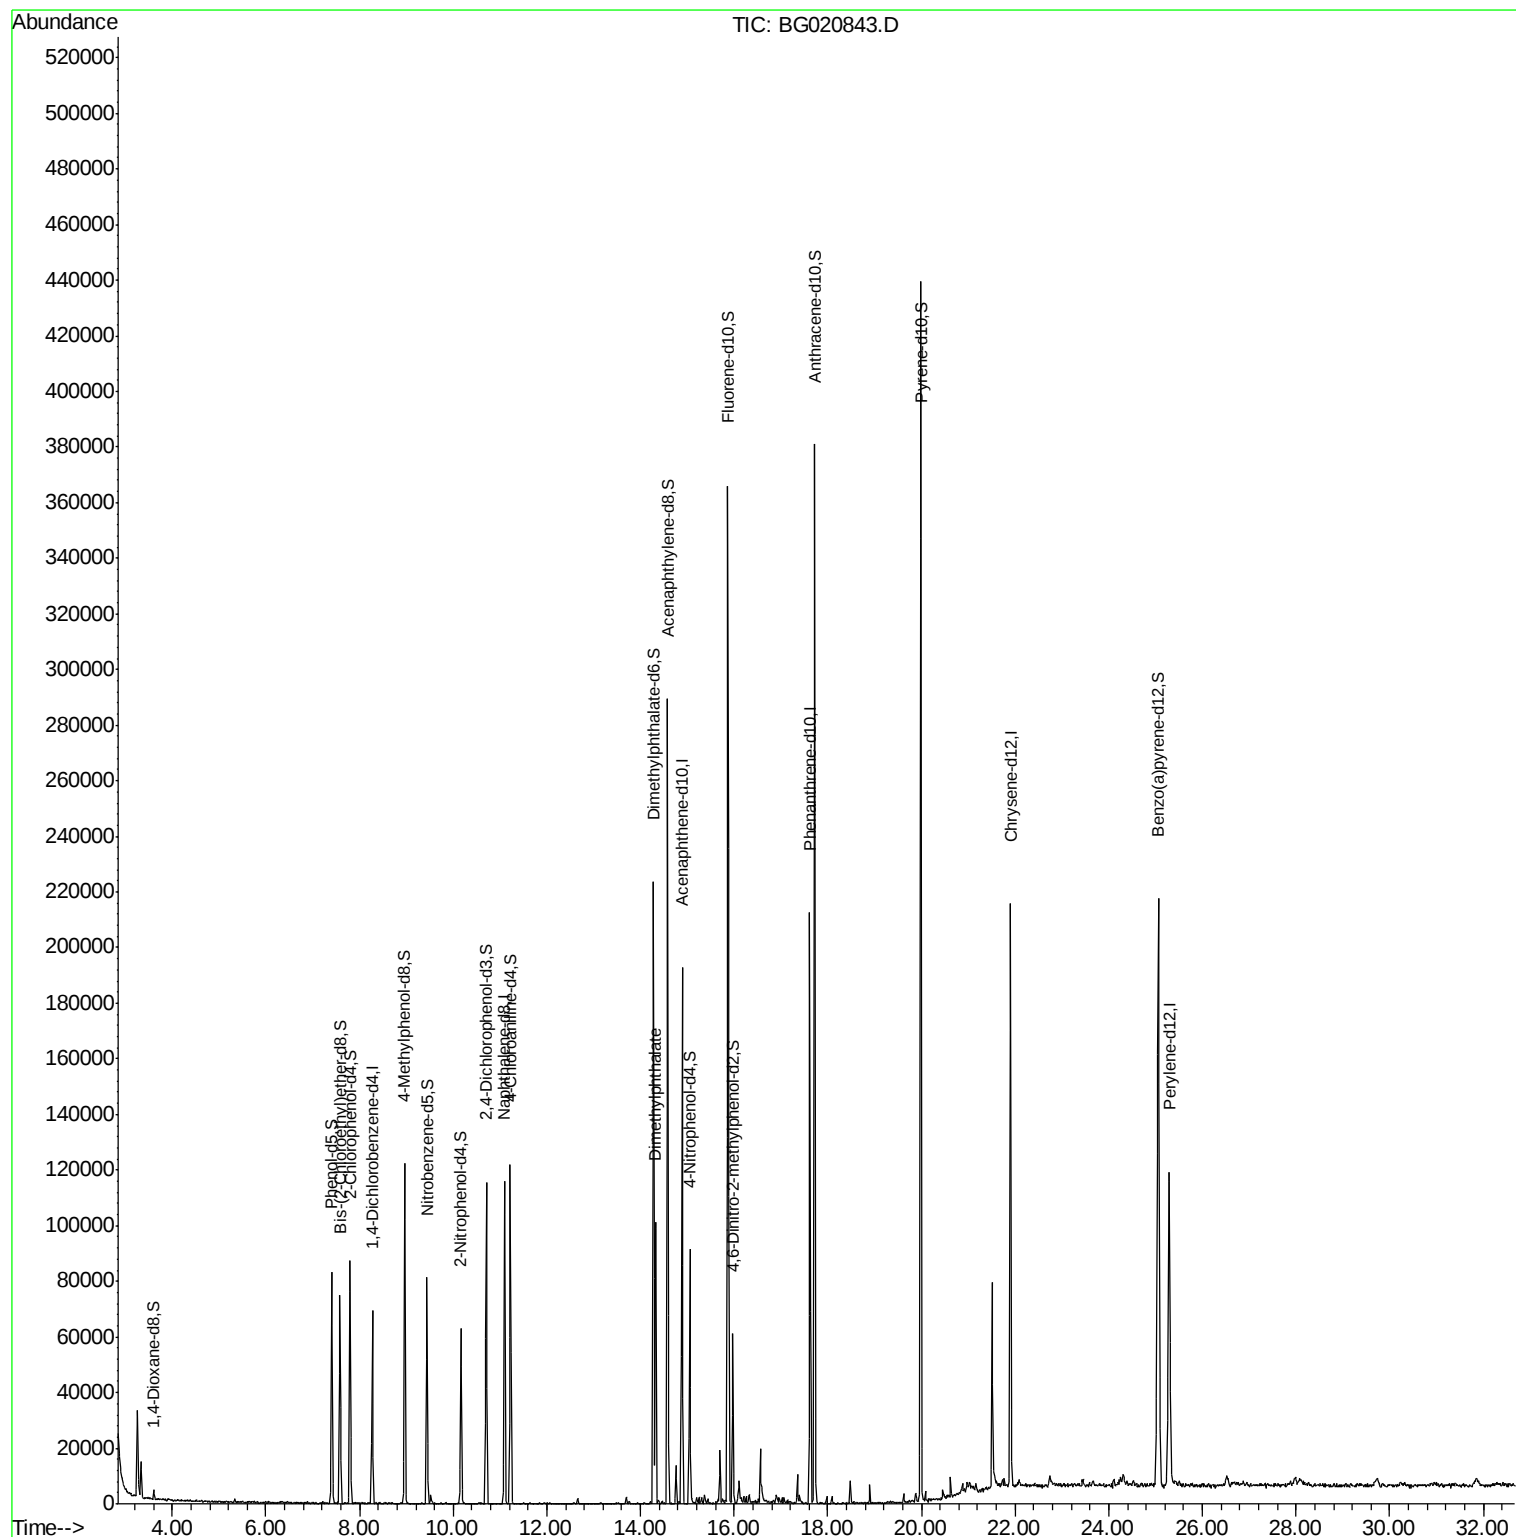

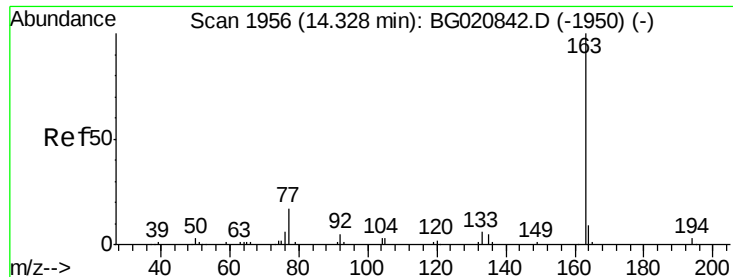

#45

Dimethylphthalate

Concen: 12.77 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. 0.00 min

Lab File: BG020843.D

Acq: 10 Feb 2016 16:42

Instrument :

BNA_G

ClientSampleId :

C04Q1


Tgt Ion:163 Resp: 73603

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 10.0 7.7 11.5

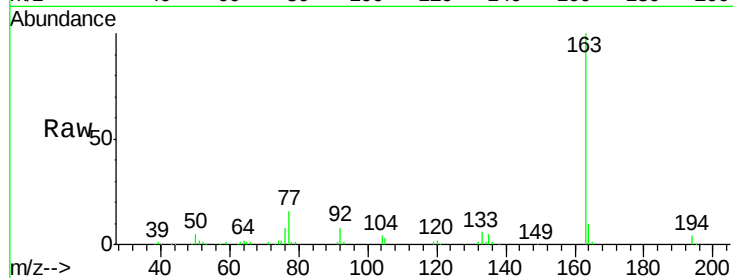

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

