

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
 Data File : BG020846.D
 Acq On : 10 Feb 2016 18:40
 Operator : SJ/UM
 Sample : H1371-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04Q4

Quant Time: Feb 11 04:07:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 11 04:03:47 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	21120	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	111346	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	62313	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	122303	20.00	ng/ul	0.00
78) Chrysene-d12	21.91	240	112987	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	105747	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	403	0.93	ng/uL	0.00
5) Phenol-d5	7.41	99	13448	6.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	32057	28.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	39684	23.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	27518	14.80	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	26899	30.11	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	27819	31.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	47827	27.96	ng/ul	0.00
29) 4-Chloroaniline-d4	11.23	131	1193	0.52	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	159300	29.71	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	207621	31.70	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	5394	5.02	ng/ul	0.00
58) Fluorene-d10	15.87	176	138294	30.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	15607	26.33	ng/ul	0.00
71) Anthracene-d10	17.72	188	186666	30.89	ng/ul	0.00
79) Pyrene-d10	19.98	212	185608	31.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	177469	30.28	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	14.32	163	8096	1.45 ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
Data File : BG020846.D
Acq On : 10 Feb 2016 18:40
Operator : SJ/UM
Sample : H1371-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04Q4

Quant Time: Feb 11 04:07:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 11 04:03:47 2016
Response via : Initial Calibration

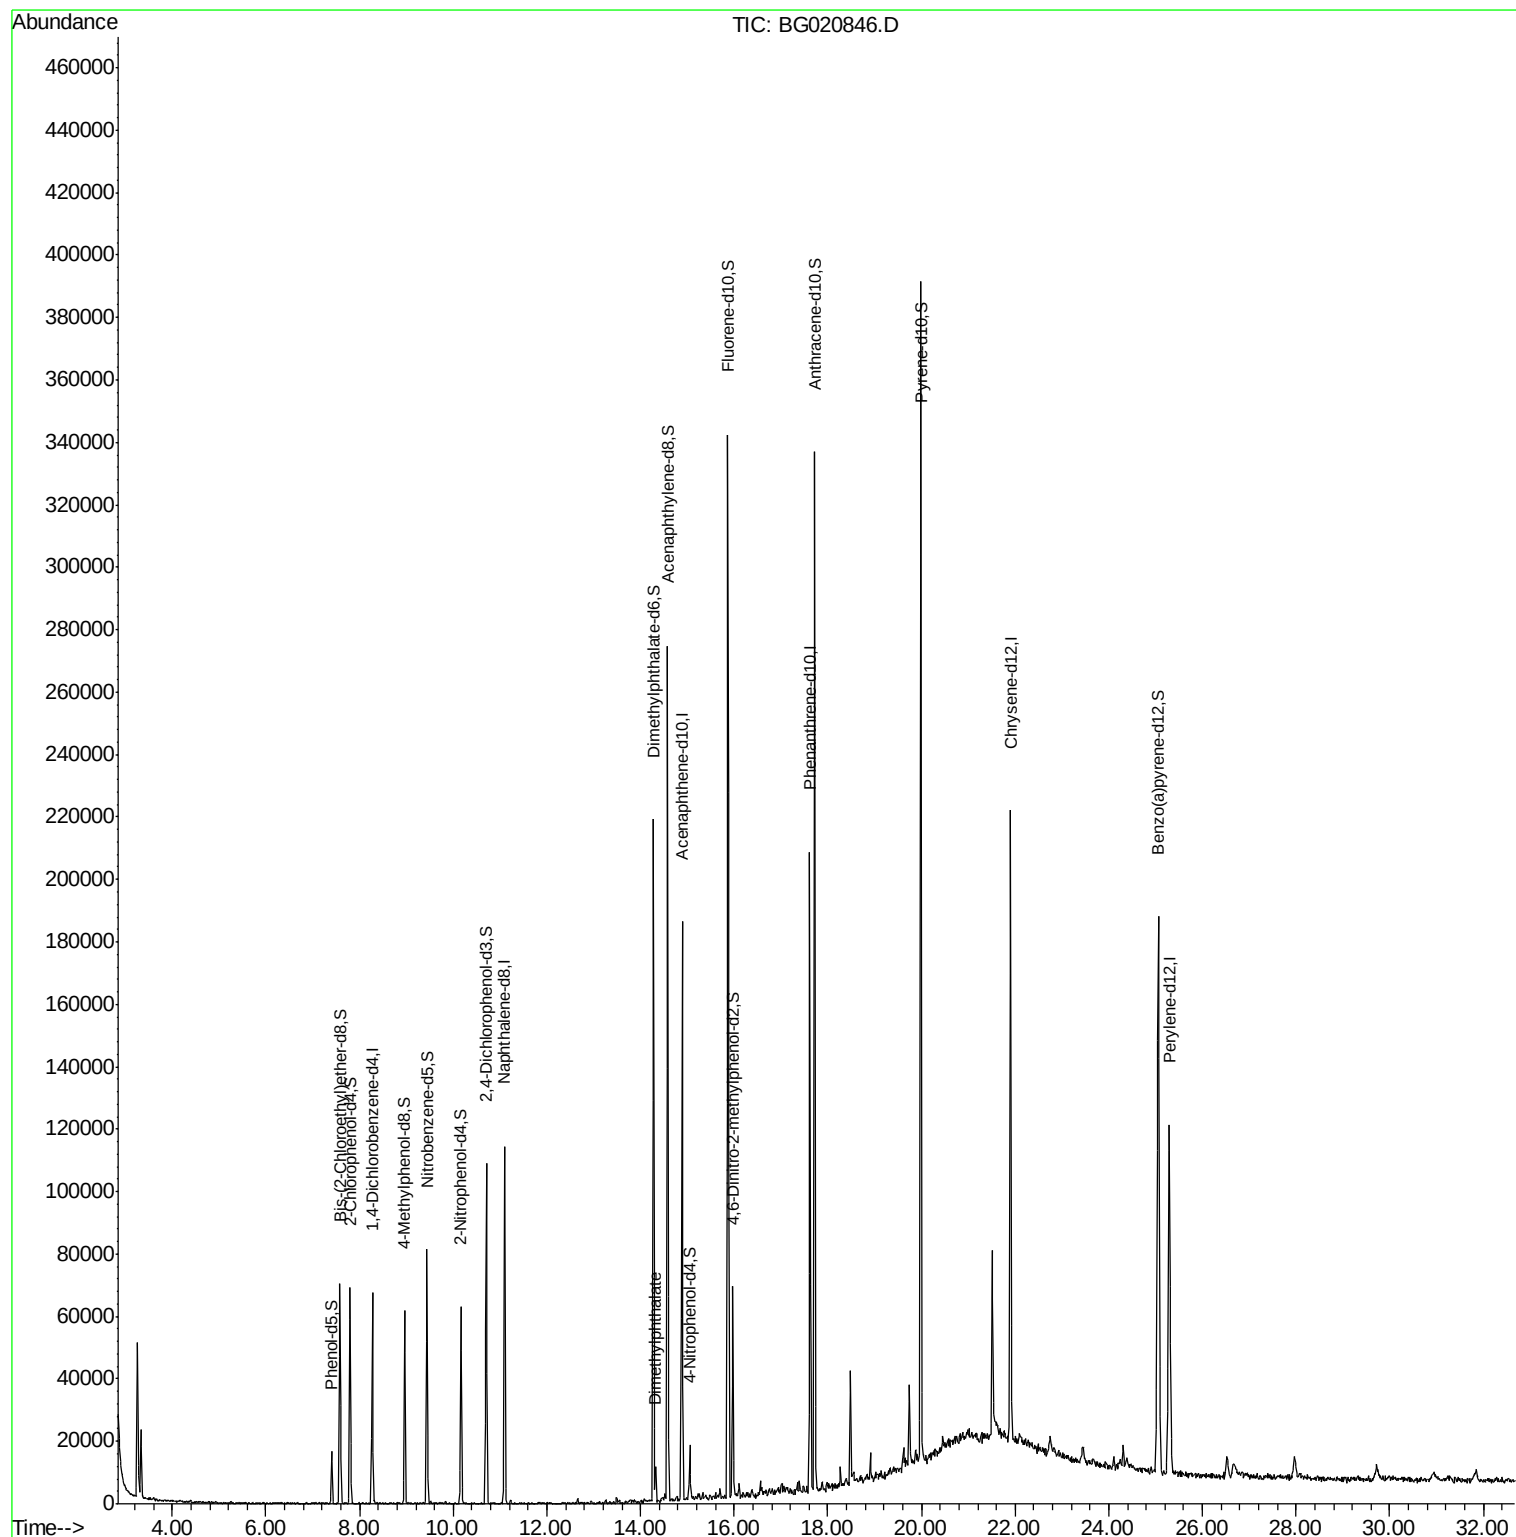

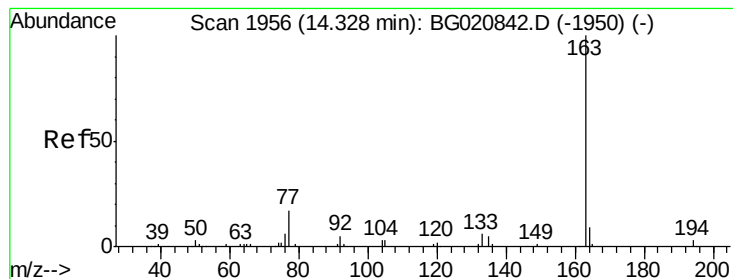

#45

Dimethylphthalate

Concen: 1.45 ng/ul

RT: 14.32 min Scan# 1955

Delta R.T. -0.01 min

Lab File: BG020846.D


Acq: 10 Feb 2016 18:40

Instrument :

BNA_G

ClientSampleId :

C04Q4

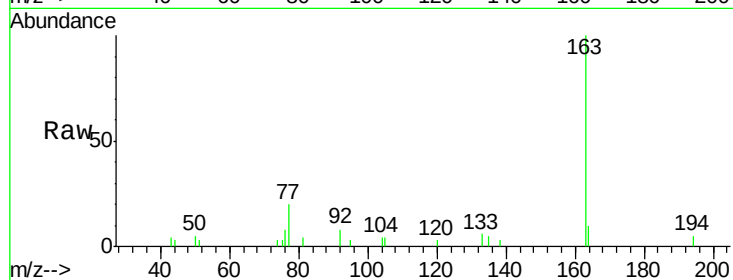

Tgt Ion:	163	Resp:	8096
Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.0	4.6#
164	9.6	7.7	11.5

