

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
 Data File : BG020838.D
 Acq On : 10 Feb 2016 13:26
 Operator : SJ/UM
 Sample : H1390-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04H3

Quant Time: Feb 11 03:29:53 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 11 03:24:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	20903	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	106492	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	63053	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	122086	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	108907	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	101023	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2664	6.19	ng/uL	0.00
5) Phenol-d5	7.40	99	66870	31.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	37114	32.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	55875	33.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	57618	31.30	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	30083	35.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	30664	36.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	54716	33.45	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	81524	37.43	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	179210	33.03	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	230835	34.83	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	30738	28.30	ng/ul	0.00
58) Fluorene-d10	15.87	176	155001	33.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.98	200	15941	26.94	ng/ul	0.00
71) Anthracene-d10	17.72	188	218006	36.14	ng/ul	0.00
79) Pyrene-d10	19.99	212	209991	37.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	203877	36.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.32	163	68588	12.14	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
Data File : BG020838.D
Acq On : 10 Feb 2016 13:26
Operator : SJ/UM
Sample : H1390-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04H3

Quant Time: Feb 11 03:29:53 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 11 03:24:50 2016
Response via : Initial Calibration

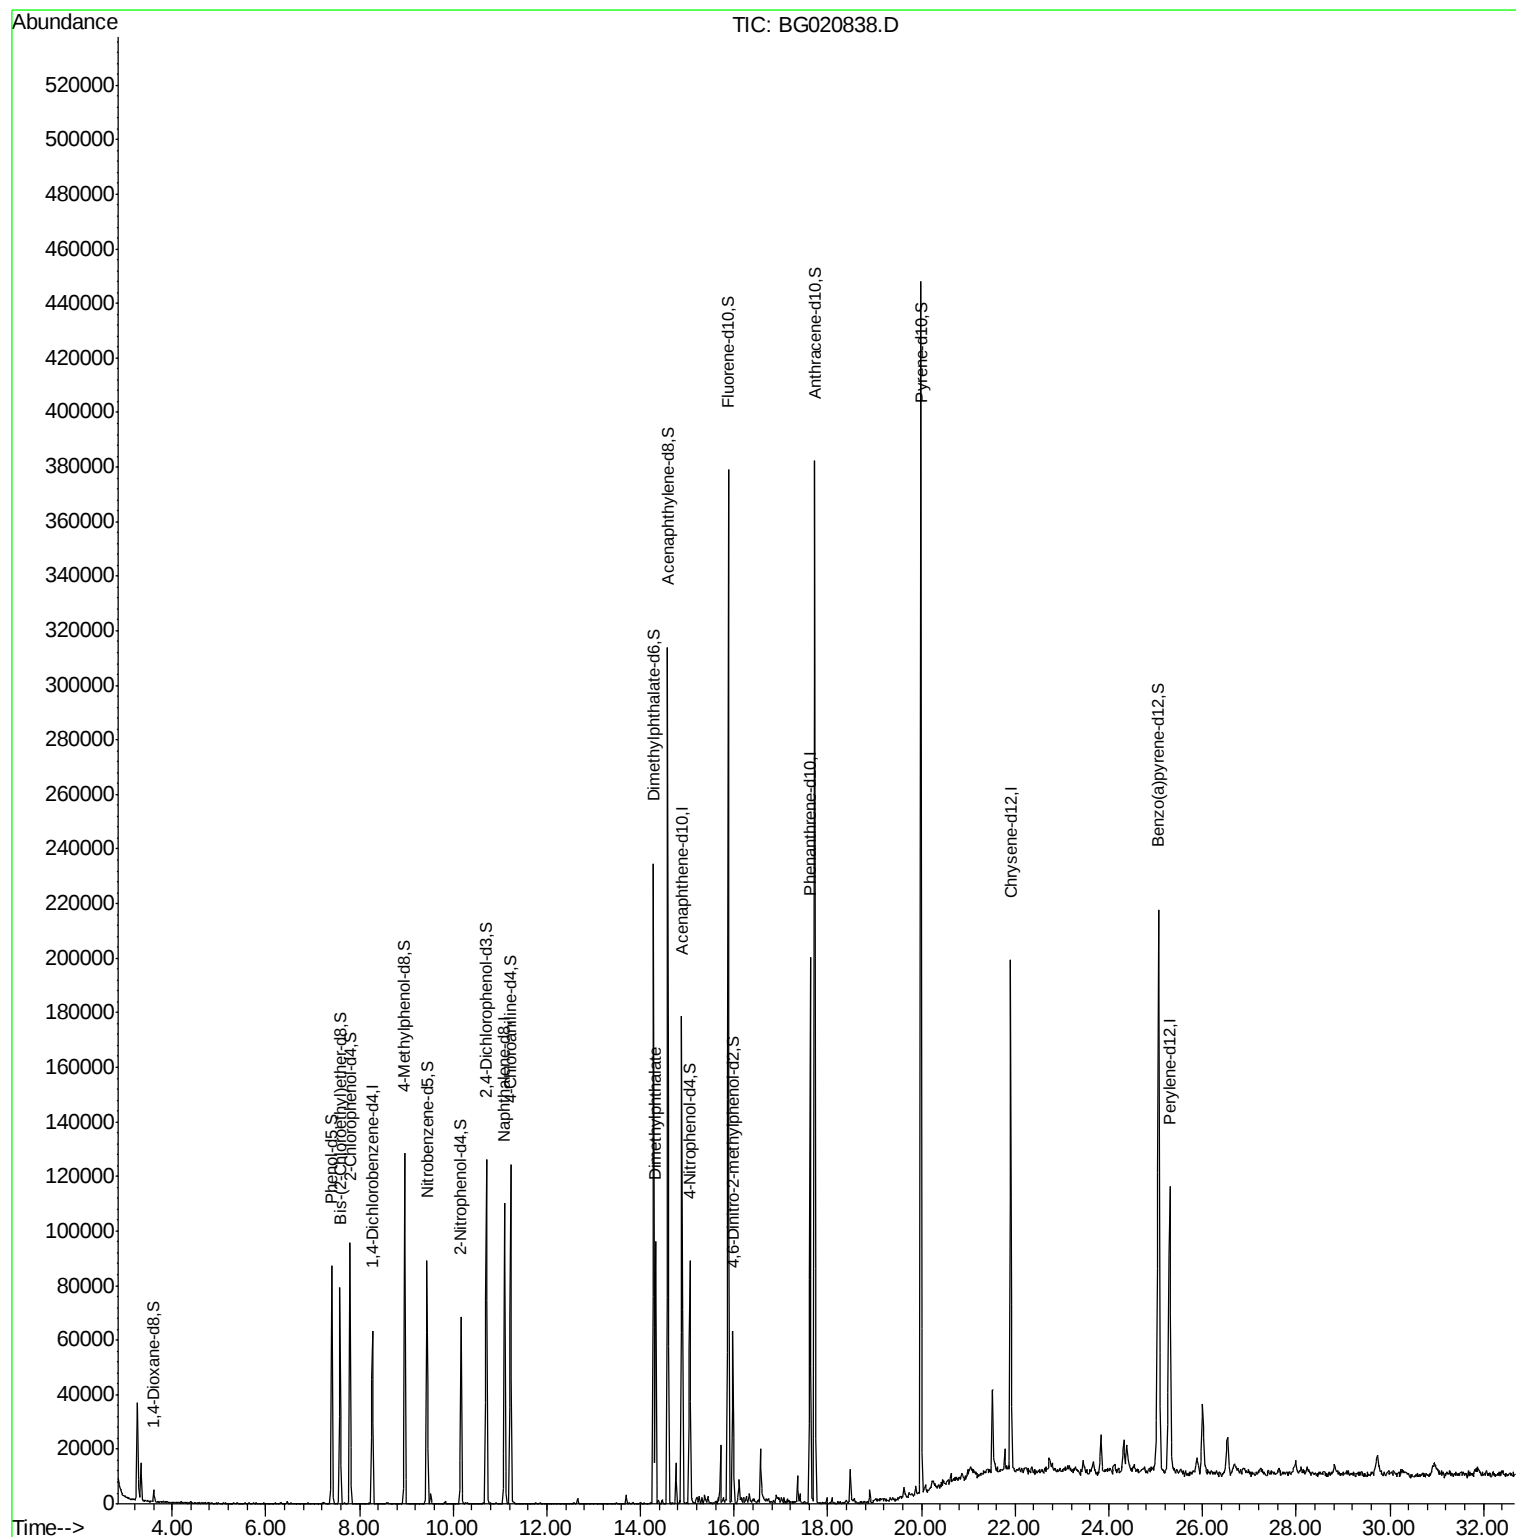

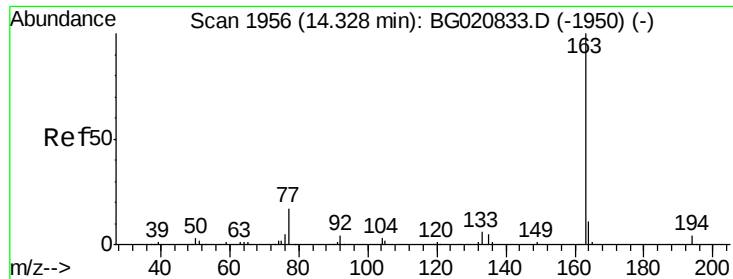

#45

Dimethylphthalate

Concen: 12.14 ng/ul

RT: 14.32 min Scan# 1955

Delta R.T. -0.00 min

Lab File: BG020838.D

Acq: 10 Feb 2016 13:26

Instrument :

BNA_G

ClientSampleId :

C04H3


Tgt Ion:163 Resp: 68588

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 10.8 7.7 11.5

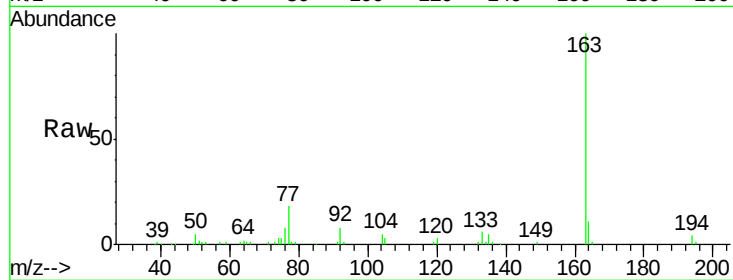

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

