

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
 Data File : BG020844.D
 Acq On : 10 Feb 2016 17:22
 Operator : SJ/UM
 Sample : H1390-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04J4

Quant Time: Feb 11 04:07:15 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 11 04:03:47 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	19769	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	101674	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	61257	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	123240	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	115139	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	107969	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2068	5.08	ng/uL	0.00
5) Phenol-d5	7.41	99	53850	26.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	29700	27.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	44310	28.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	49277	28.31	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	24137	29.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	25540	31.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	44669	28.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	71418	34.34	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	157728	29.92	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	199767	31.02	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	26750	25.35	ng/ul	0.00
58) Fluorene-d10	15.87	176	137285	30.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	13027	21.81	ng/ul	0.00
71) Anthracene-d10	17.72	188	197712	32.47	ng/ul	0.00
79) Pyrene-d10	19.98	212	196242	33.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	190606	31.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.33	163	58720	10.70	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021016\
Data File : BG020844.D
Acq On : 10 Feb 2016 17:22
Operator : SJ/UM
Sample : H1390-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04J4

Quant Time: Feb 11 04:07:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 11 04:03:47 2016
Response via : Initial Calibration

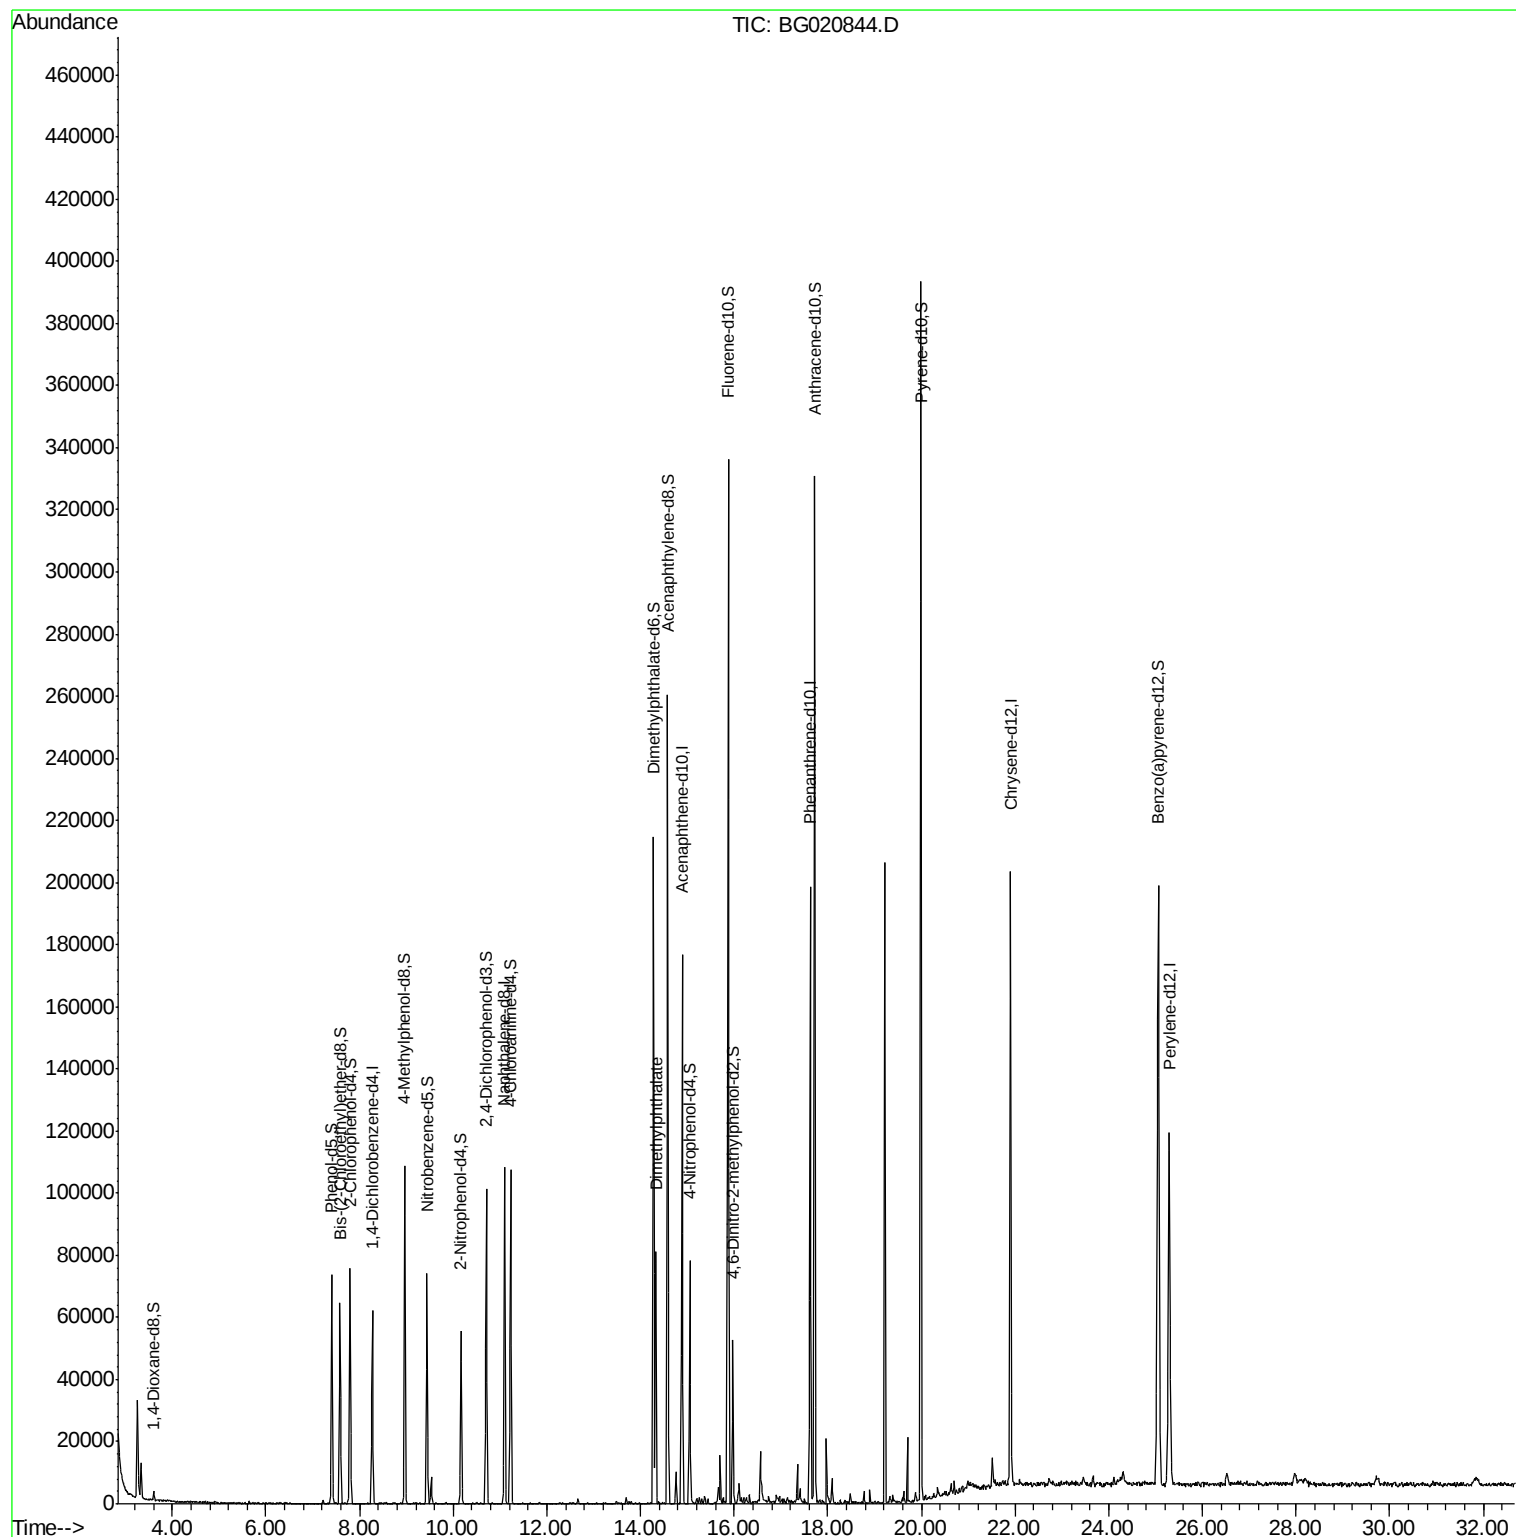

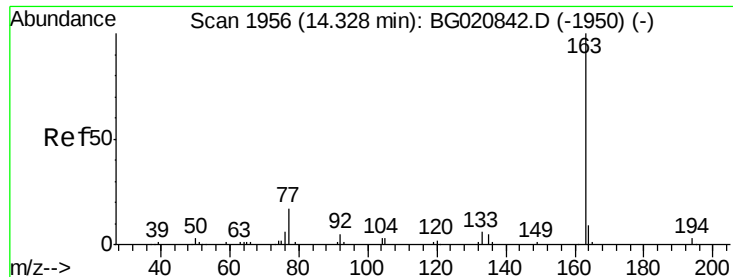

#45

Dimethylphthalate

Concen: 10.70 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. -0.00 min

Lab File: BG020844.D

Acq: 10 Feb 2016 17:22

Instrument :

BNA_G

ClientSampleId :

C04J4


Tgt Ion:163 Resp: 58720

Ion Ratio Lower Upper

163 100

194 4.3 3.0 4.6

164 10.4 7.7 11.5

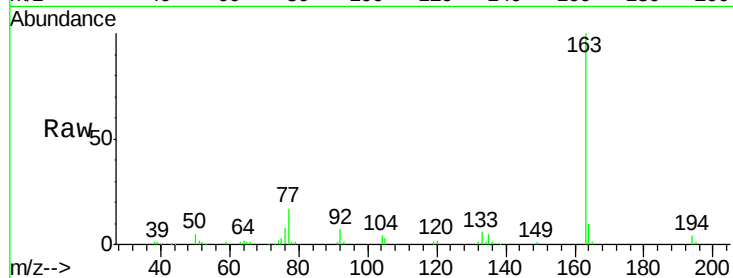

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

