

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
 Data File : BG052349.D
 Acq On : 10 Feb 2022 11:08
 Operator : CG/JU
 Sample : PB142553BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB142553BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.761	380	387	403	rVB	519462	822393	23.91%	7.501%
2	7.382	655	663	673	rBV	543870	938592	27.29%	8.561%
3	8.234	801	808	818	rVB	73131	123178	3.58%	1.124%
4	9.409	997	1008	1019	rBV	336422	610477	17.75%	5.568%
5	11.071	1284	1291	1300	rBV	107977	194672	5.66%	1.776%
6	13.503	1697	1705	1713	rBV	968106	1540974	44.80%	14.056%
7	14.878	1932	1939	1950	rVB	210928	323856	9.41%	2.954%
8	16.364	2184	2192	2201	rBV	917065	1384118	40.24%	12.625%
9	17.627	2400	2407	2417	rVB	306770	474049	13.78%	4.324%
10	20.218	2842	2848	2854	rBV	2556611	3439896	100.00%	31.377%
11	21.939	3134	3141	3149	rVB	335062	550787	16.01%	5.024%
12	25.417	3722	3733	3747	rVB2	174944	560103	16.28%	5.109%




Sum of corrected areas: 10963095

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052349.D
Acq On : 10 Feb 2022 11:08
Operator : CG/JU
Sample : PB142553BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142553BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

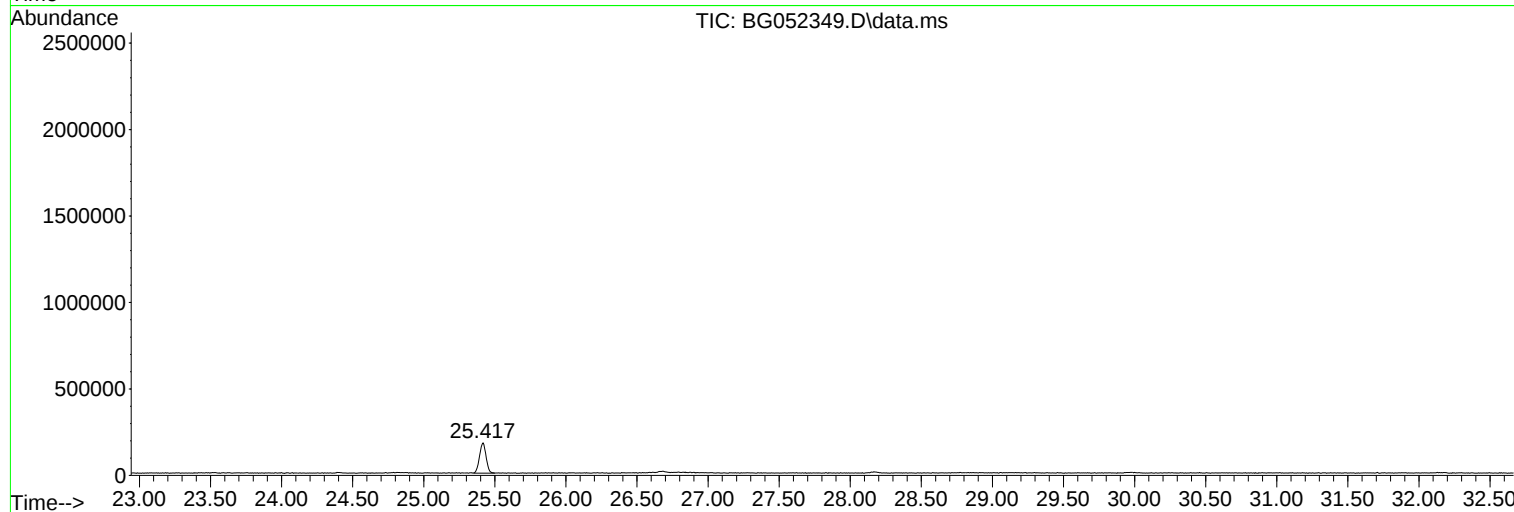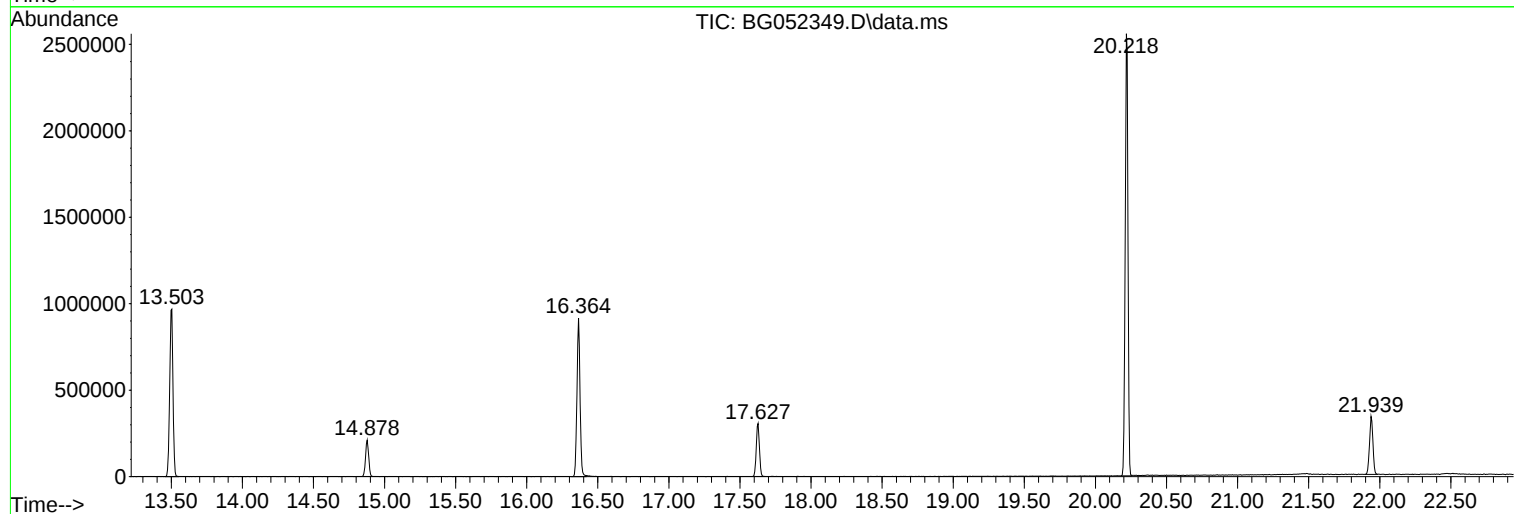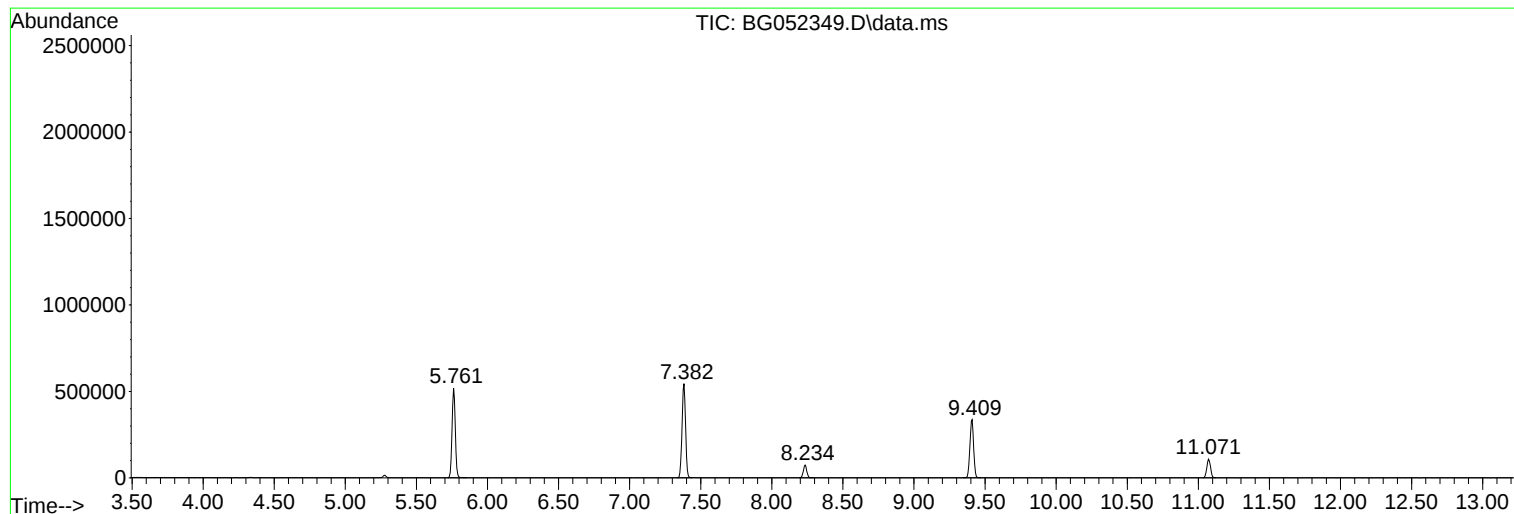

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052349.D
Acq On : 10 Feb 2022 11:08
Operator : CG/JU
Sample : PB142553BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142553BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052349.D
Acq On : 10 Feb 2022 11:08
Operator : CG/JU
Sample : PB142553BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142553BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------