

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
 Data File : BG052352.D
 Acq On : 10 Feb 2022 13:42
 Operator : CG/JU
 Sample : PB142486BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB142486BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.756	379	386	401	rBV	519803	824314	23.96%	7.426%
2	7.372	650	661	674	rBV	547231	956312	27.80%	8.616%
3	8.223	801	806	813	rVB	72321	122414	3.56%	1.103%
4	9.398	998	1006	1017	rVB	342544	610681	17.75%	5.502%
5	11.067	1282	1290	1298	rBV	110064	198729	5.78%	1.790%
6	13.499	1696	1704	1712	rBV	996334	1564763	45.49%	14.097%
7	14.873	1930	1938	1945	rBV	210672	330472	9.61%	2.977%
8	16.359	2184	2191	2203	rBV	881879	1395437	40.57%	12.572%
9	17.622	2400	2406	2417	rVB	320280	481987	14.01%	4.342%
10	20.219	2842	2848	2855	rBV	2635355	3439760	100.00%	30.990%
11	21.464	3051	3060	3071	rBV6	16186	54271	1.58%	0.489%
12	21.940	3134	3141	3149	rVB	318719	554491	16.12%	4.996%
13	25.412	3719	3732	3747	rBV	180215	566036	16.46%	5.100%




Sum of corrected areas: 11099667

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052352.D
Acq On : 10 Feb 2022 13:42
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

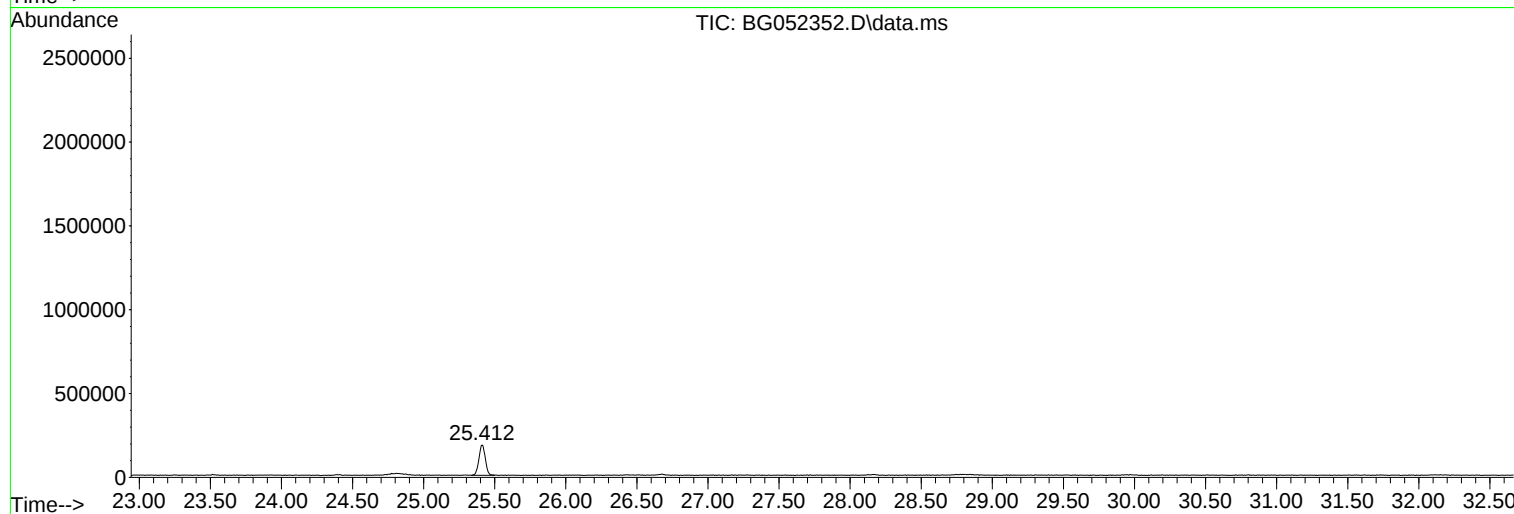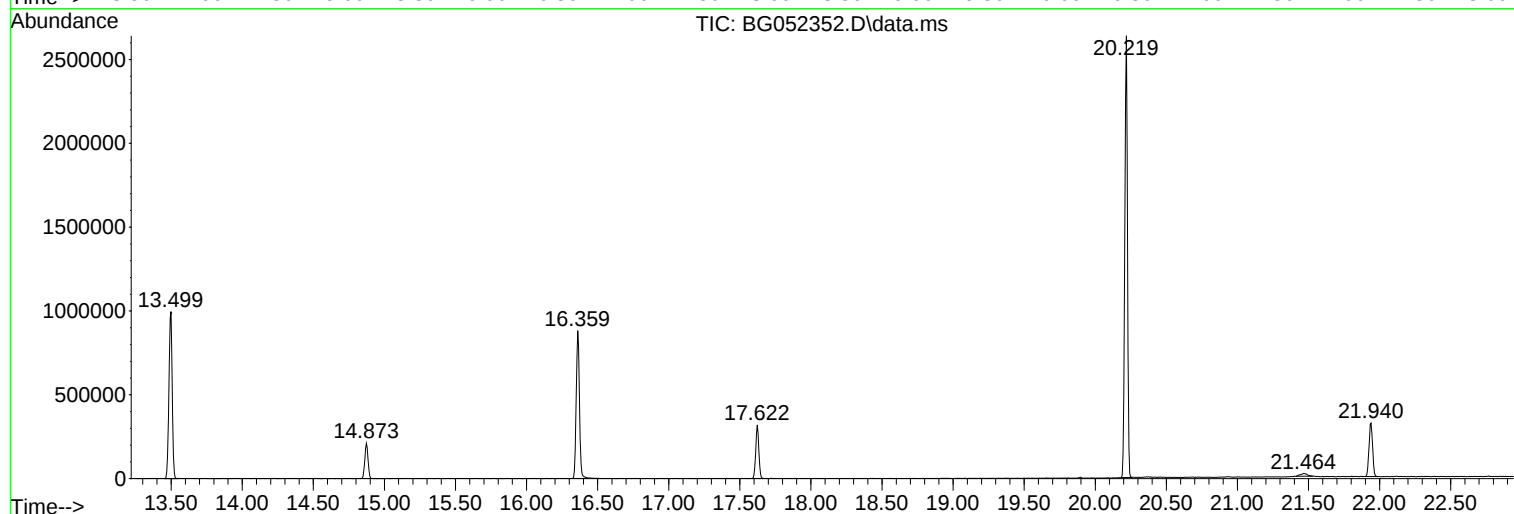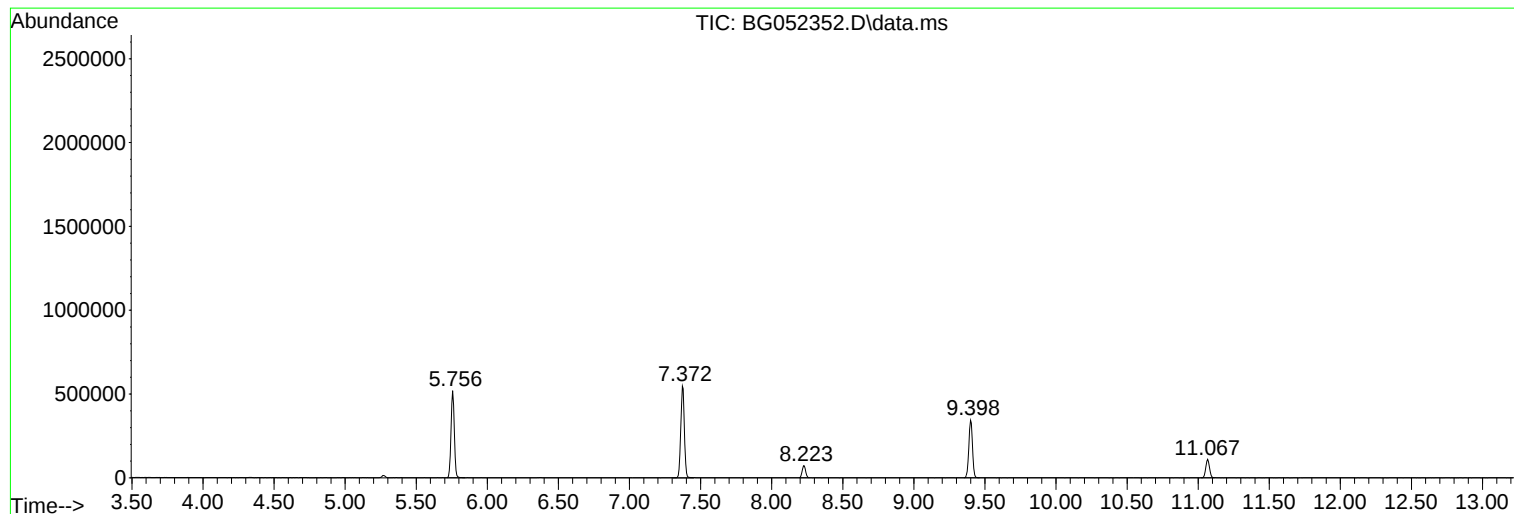

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052352.D
Acq On : 10 Feb 2022 13:42
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052352.D
Acq On : 10 Feb 2022 13:42
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------