

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
 Data File : BG052357.D
 Acq On : 10 Feb 2022 17:00
 Operator : CG/JU
 Sample : N1432-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.756	378	386	395	rBV	485146	762382	35.95%	8.305%
2	7.372	654	661	673	rBV	484666	839273	39.58%	9.143%
3	8.224	800	806	813	rBV	98599	165415	7.80%	1.802%
4	9.398	997	1006	1014	rBV	307930	540238	25.48%	5.885%
5	11.067	1281	1290	1300	rVB	123658	233545	11.01%	2.544%
6	13.493	1696	1703	1712	rVB	792158	1216971	57.39%	13.257%
7	14.873	1931	1938	1946	rVB	218776	341525	16.11%	3.720%
8	16.360	2184	2191	2203	rBV	672531	1067809	50.36%	11.632%
9	17.623	2398	2406	2411	rBV	303827	462506	21.81%	5.038%
10	18.486	2549	2553	2559	rBV7	13542	22877	1.08%	0.249%
11	20.213	2841	2847	2853	rVB	1621127	2120390	100.00%	23.098%
12	21.000	2977	2981	2985	rVB3	20253	25807	1.22%	0.281%
13	21.529	3067	3071	3082	rVB3	64320	106907	5.04%	1.165%
14	21.934	3133	3140	3147	rBV2	297158	527394	24.87%	5.745%
15	22.117	3166	3171	3177	rVB2	28545	39742	1.87%	0.433%
16	22.769	3278	3282	3289	rVB2	23085	36419	1.72%	0.397%
17	23.515	3404	3409	3421	rVB2	23974	49459	2.33%	0.539%
18	24.396	3554	3559	3565	rVB4	24403	52509	2.48%	0.572%
19	25.412	3720	3732	3745	rBV	179754	568677	26.82%	6.195%




Sum of corrected areas: 9179845

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052357.D
Acq On : 10 Feb 2022 17:00
Operator : CG/JU
Sample : N1432-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

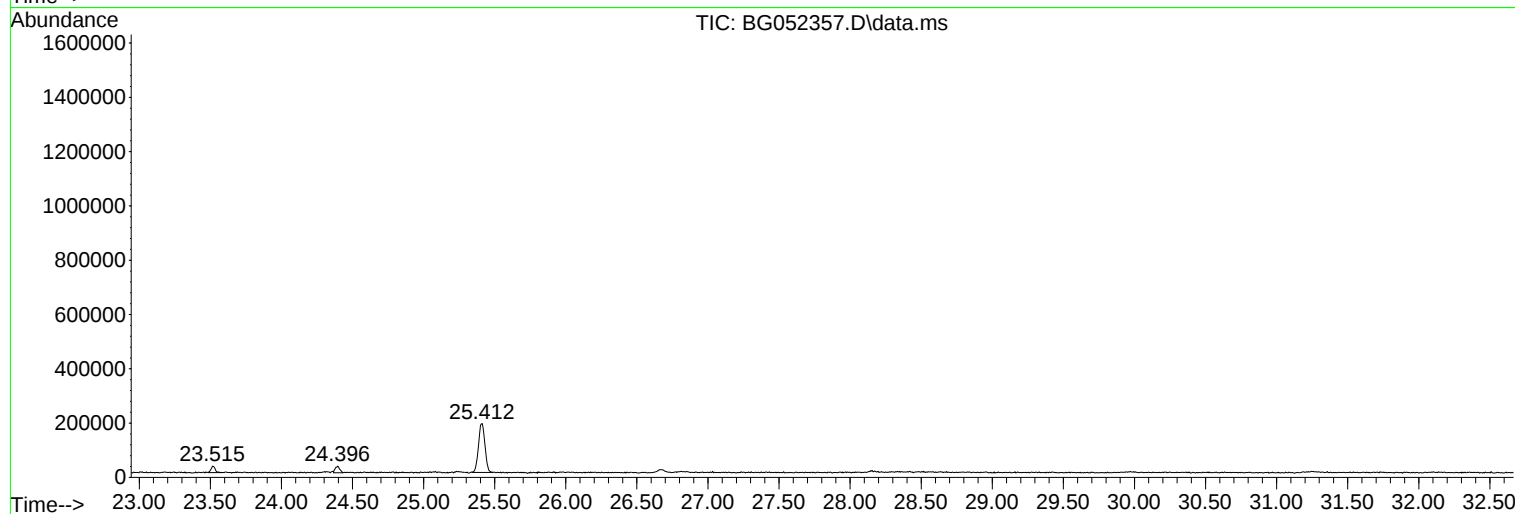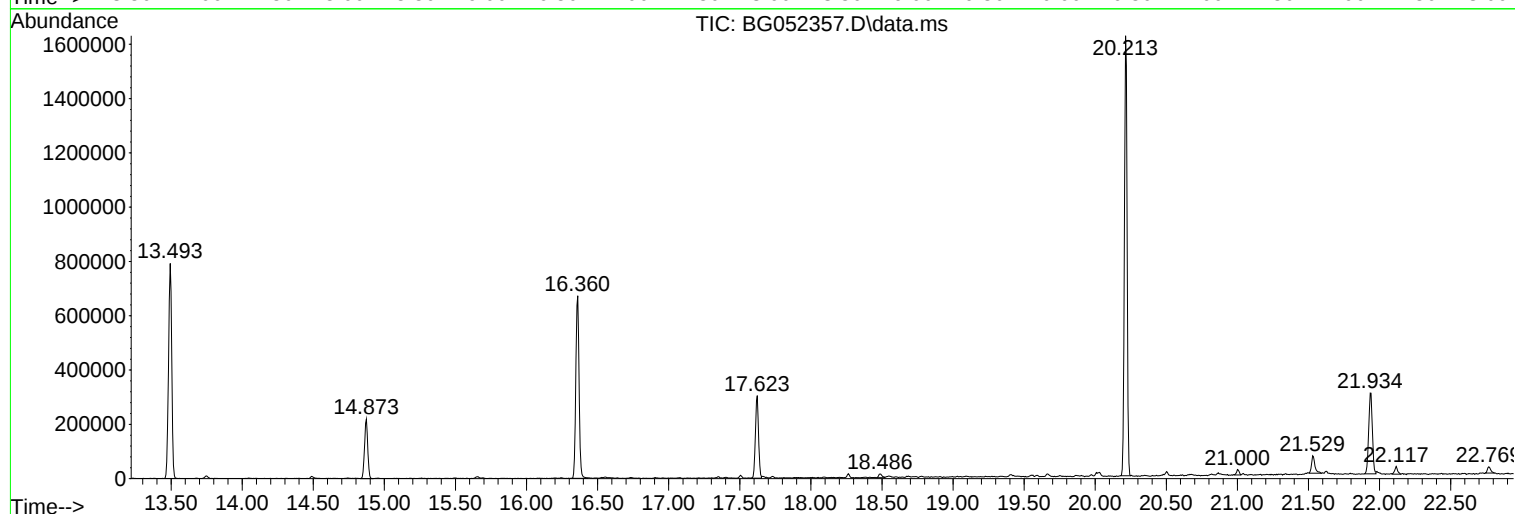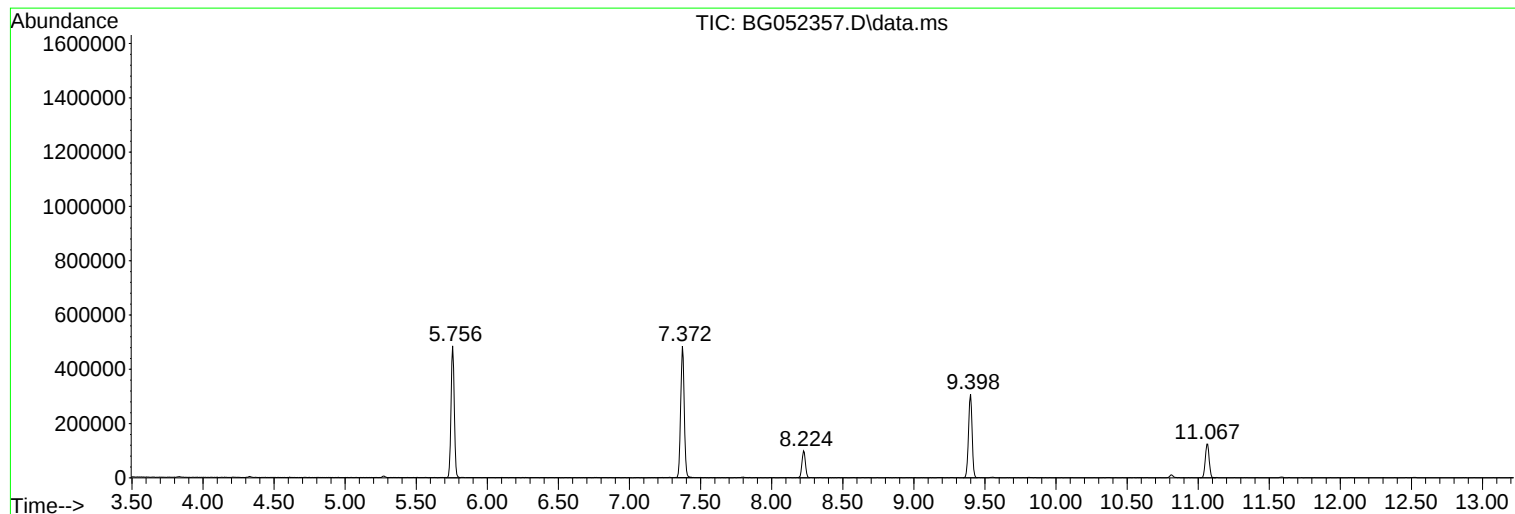

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052357.D
Acq On : 10 Feb 2022 17:00
Operator : CG/JU
Sample : N1432-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 17-Pentatriacontene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.529	4.05 ng	106907	Chrysene-d12	21.940

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			17-Pentatriacontene	491	C35H70	006971-40-0	91
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
3			1-Hexadecanesulfonyl chloride	324	C16H33ClO2S	038775-38-1	91
4			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	87
5			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	87

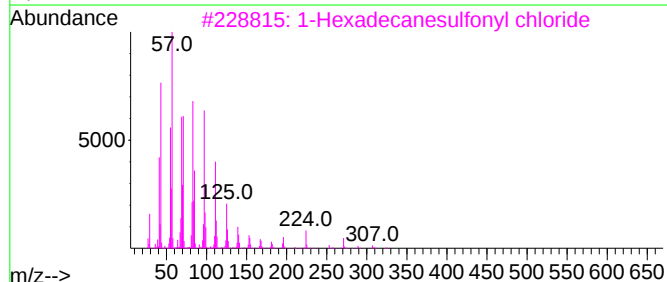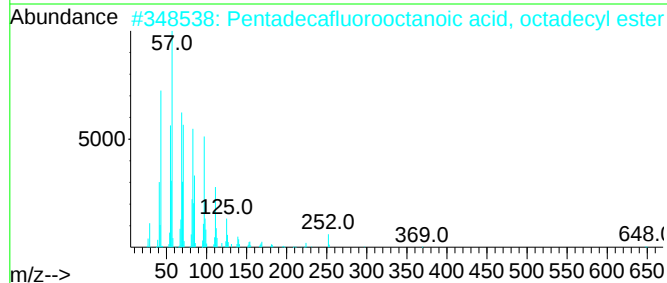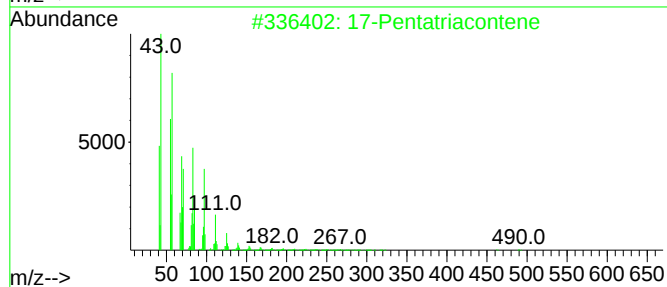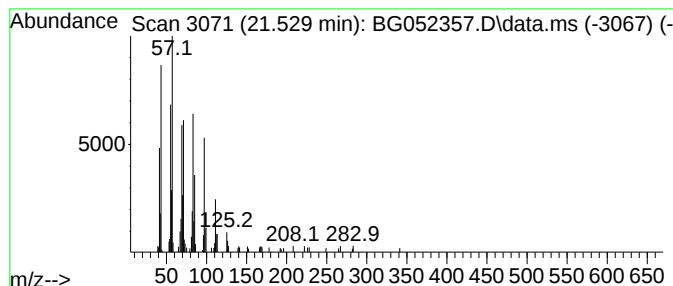

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021022\
Data File : BG052357.D
Acq On : 10 Feb 2022 17:00
Operator : CG/JU
Sample : N1432-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
17-Pentatriacon...	21.529	4.0	ng	106907	5	21.940	527394	20.0