

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
 Data File : BG056616.D
 Acq On : 10 Feb 2023 22:07
 Operator : CG/JU
 Sample : 01328-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1-BORING-1-0-7

Quant Time: Feb 10 23:30:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 10 22:46:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.212	152	33303	20.000	ng	# 0.00
21) Naphthalene-d8	11.044	136	135812	20.000	ng	0.00
39) Acenaphthene-d10	14.840	164	103226	20.000	ng	0.00
64) Phenanthrene-d10	17.578	188	232539	20.000	ng	0.00
76) Chrysene-d12	21.855	240	214564	20.000	ng	0.00
86) Perylene-d12	25.239	264	238030	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.739	112	278176	153.658	ng	0.01
7) Phenol-d6	7.378	99	388707	144.912	ng	0.01
23) Nitrobenzene-d5	9.393	82	200738	83.932	ng	0.00
42) 2,4,6-Tribromophenol	16.326	330	176097	128.320	ng	0.00
45) 2-Fluorobiphenyl	13.465	172	663152	89.068	ng	0.00
79) Terphenyl-d14	20.157	244	1054412	86.311	ng	0.00
Target Compounds						
						Qvalue
9) Benzaldehyde	7.384	77	522	Below Cal	#	1
19) n-Nitroso-di-n-propyla...	9.393	70	24571	15.895	ng	# 74
51) 2,6-Dinitrotoluene	14.840	165	13306	7.306	ng	# 36
57) 2,4-Dinitrotoluene	14.840	165	13306	5.187	ng	# 35
67) 4-Bromophenyl-phenylether	16.326	248	14200	4.770	ng	# 1
85) Di-n-octyl phthalate	23.024	149	90977	8.176	ng	# 43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056616.D
Acq On : 10 Feb 2023 22:07
Operator : CG/JU
Sample : 01328-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7

Quant Time: Feb 10 23:30:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration




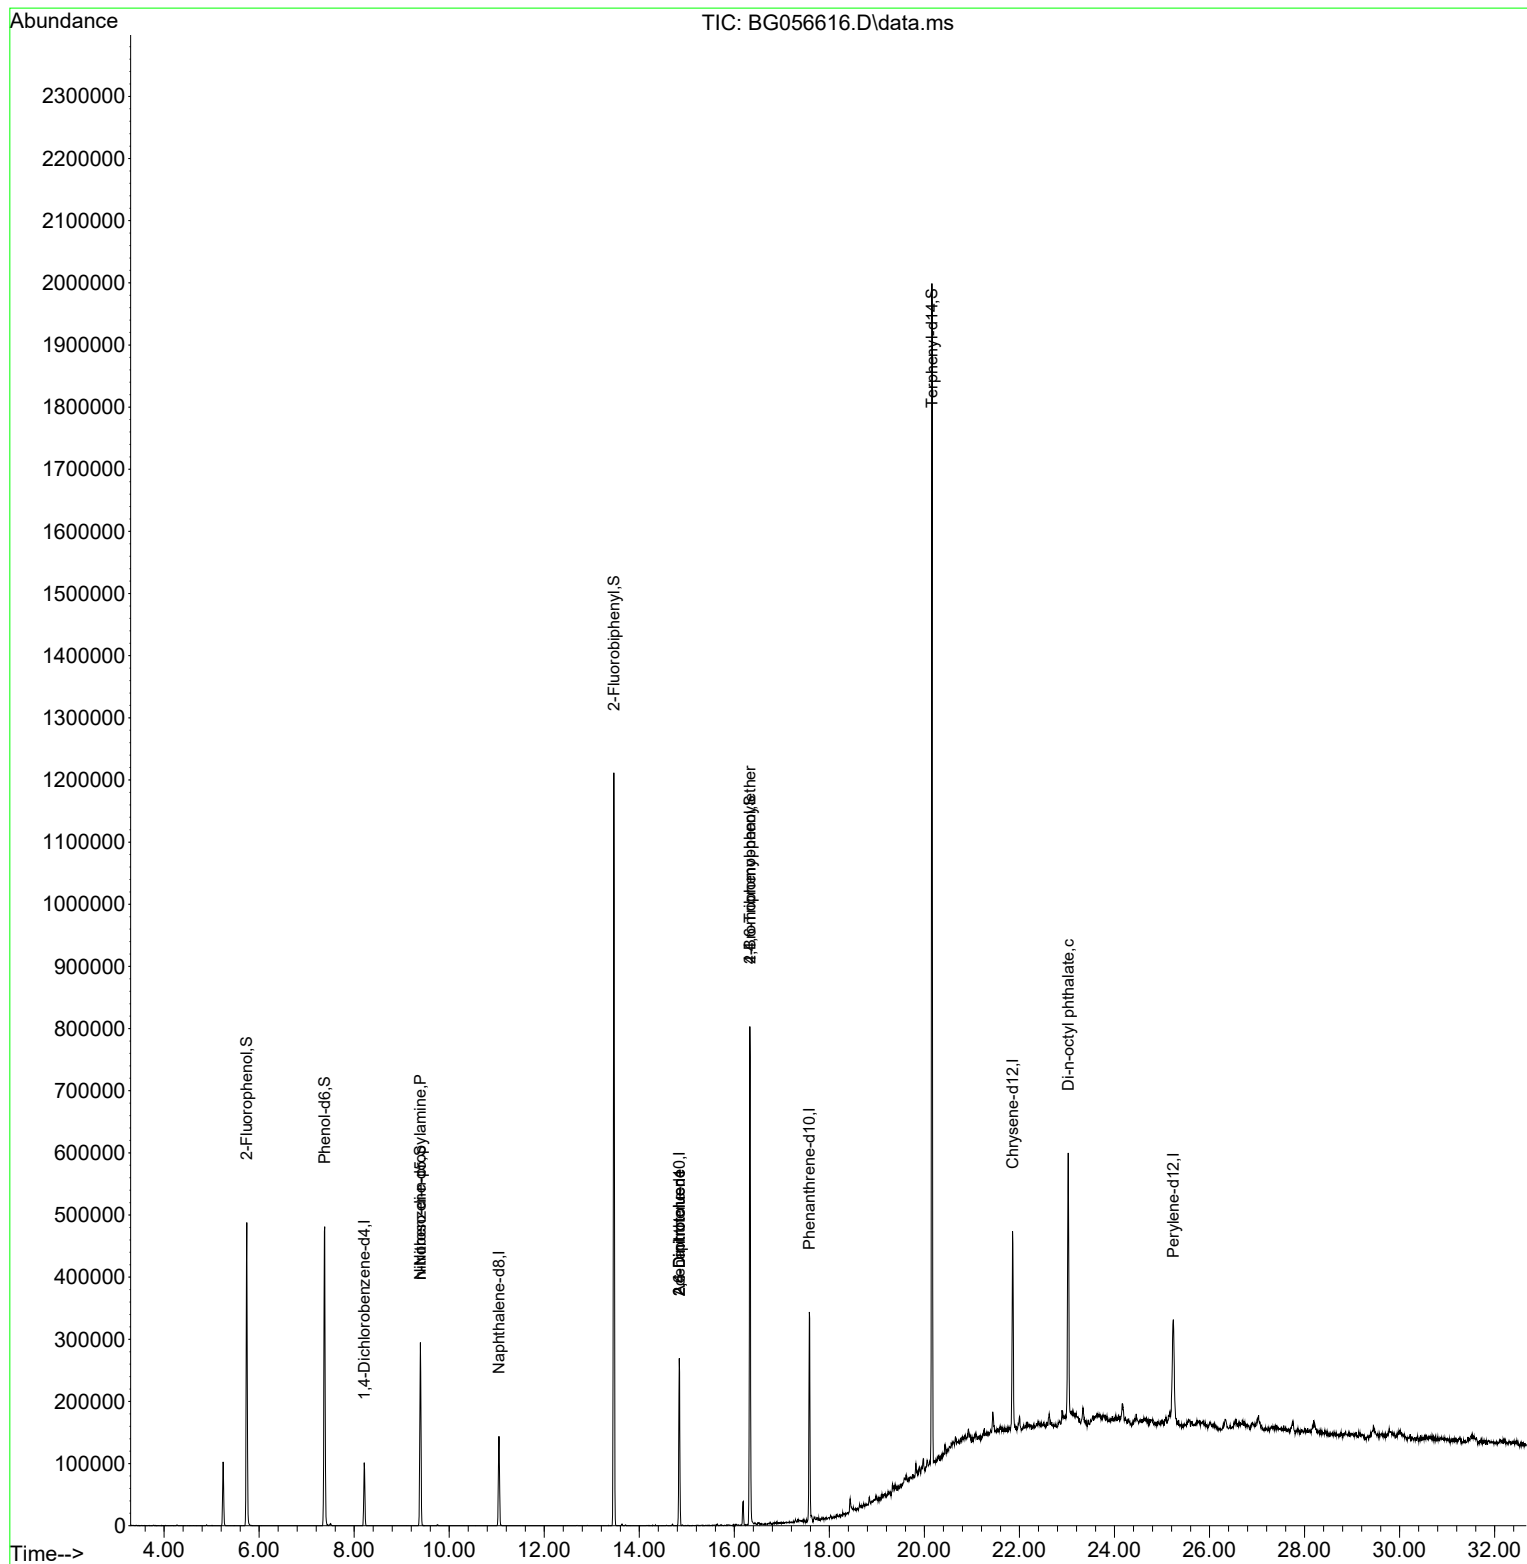




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.212 min Scan# 81
Delta R.T. 0.005 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion:152 Resp: 33303
Ion Ratio Lower Upper
152 100
150 163.4 120.2 180.4
115 56.6 36.3 54.5#

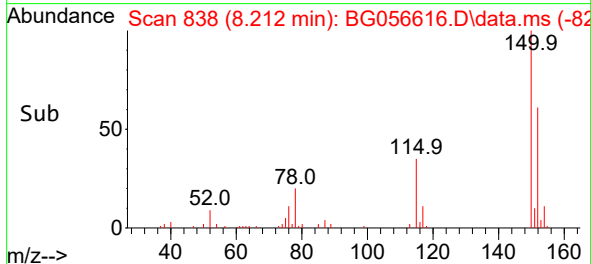

#5
2-Fluorophenol
Concen: 153.658 ng
RT: 5.739 min Scan# 417
Delta R.T. 0.011 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion:112 Resp: 278176
Ion Ratio Lower Upper
112 100
64 37.8 31.9 47.9
63 21.7 17.4 26.0


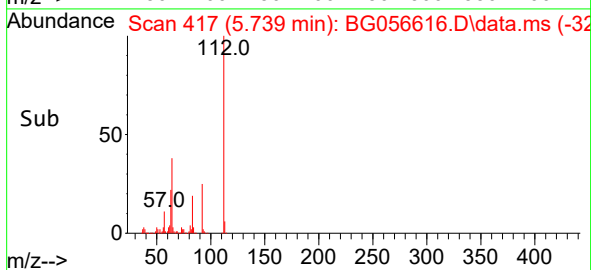

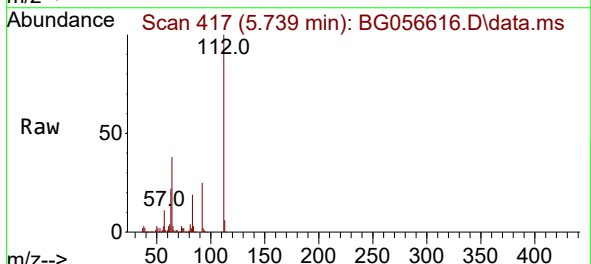




#7
Phenol-d6
Concen: 144.912 ng
RT: 7.378 min Scan# 61
Delta R.T. 0.011 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion: 99 Resp: 388707
Ion Ratio Lower Upper
99 100
42 7.5 6.6 10.0
71 28.5 23.4 35.0

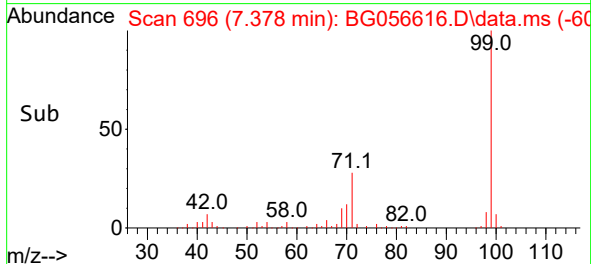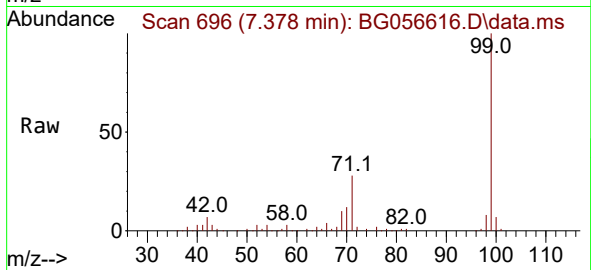

#19
n-Nitroso-di-n-propylamine
Concen: 15.895 ng
RT: 9.393 min Scan# 1039
Delta R.T. 0.375 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion: 70 Resp: 24571
Ion Ratio Lower Upper
70 100
42 26.7 20.2 30.4
101 0.0 9.1 13.7#
130 2.8 21.1 31.7#


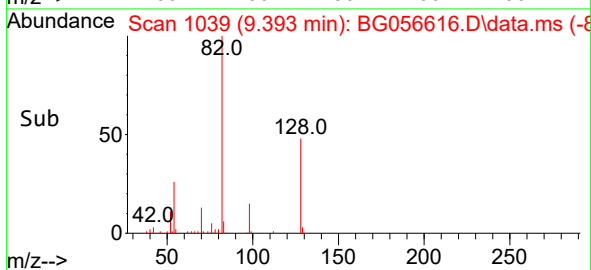

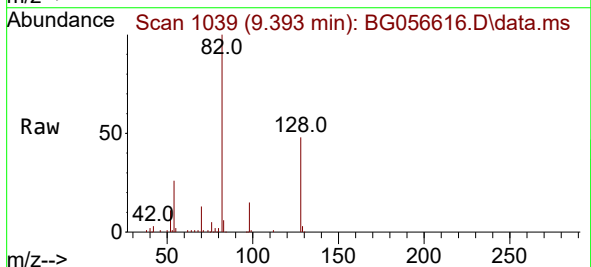




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.044 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion:136	Resp: 135812
Ion Ratio	Lower Upper
136	100
137	10.9 9.4 14.0
54	3.0 2.2 3.4
68	4.7 3.6 5.4

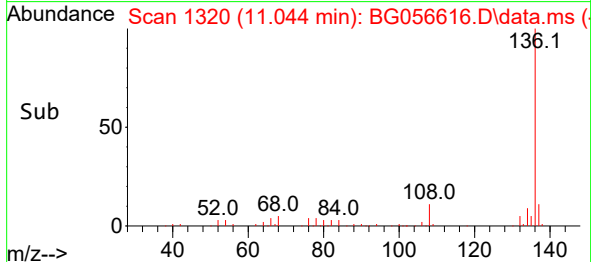

#23
Nitrobenzene-d5
Concen: 83.932 ng
RT: 9.393 min Scan# 1039
Delta R.T. 0.005 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion: 82	Resp: 200738
Ion Ratio	Lower Upper
82	100
128	47.7 39.4 59.2
54	26.3 21.4 32.2


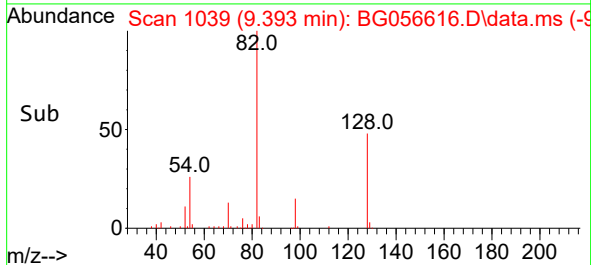

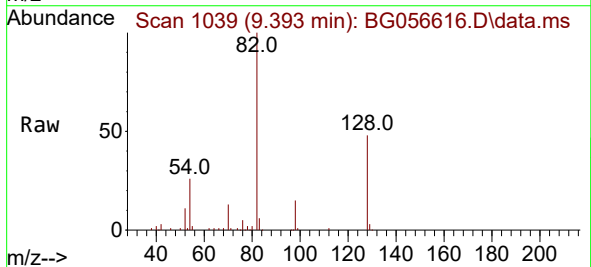




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.840 min Scan# 1977
Delta R.T. -0.001 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion:164 Resp: 103226
Ion Ratio Lower Upper
164 100
162 98.9 79.6 119.4
160 41.0 34.9 52.3

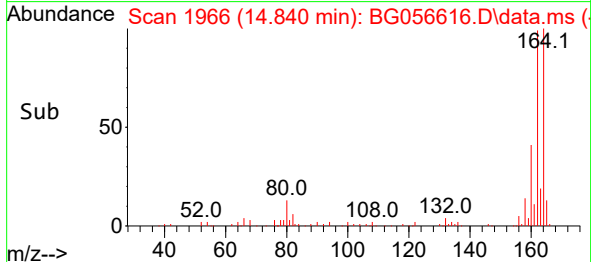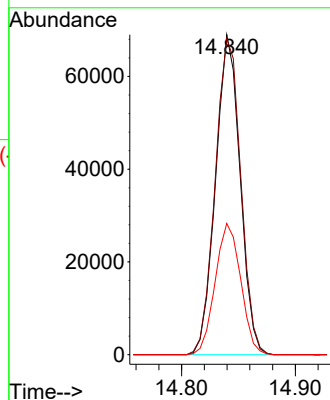

#42
2,4,6-Tribromophenol
Concen: 128.320 ng
RT: 16.326 min Scan# 2219
Delta R.T. -0.001 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion:330 Resp: 176097
Ion Ratio Lower Upper
330 100
332 97.9 79.0 118.6
141 30.8 24.2 36.4


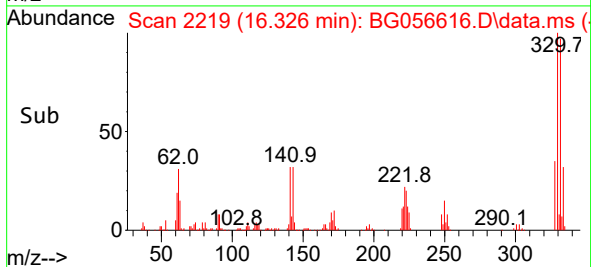
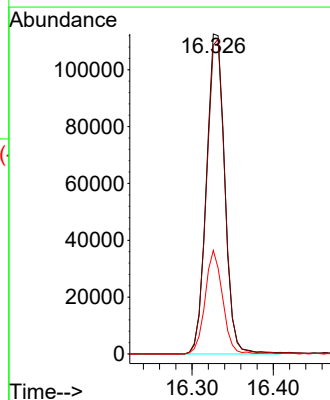
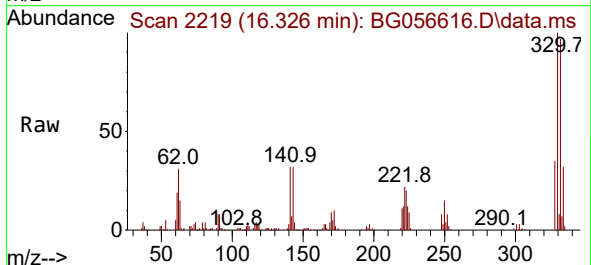




#45
2-Fluorobiphenyl
Concen: 89.068 ng
RT: 13.465 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion:172 Resp: 663152
Ion Ratio Lower Upper
172 100
171 37.3 29.5 44.3
170 25.1 19.2 28.8

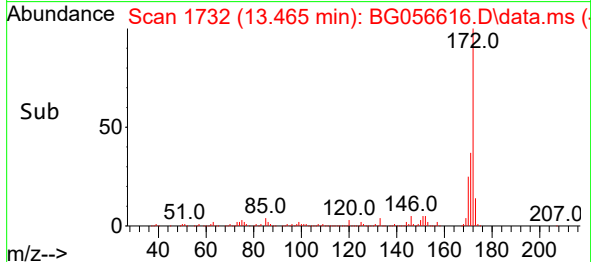

#51
2,6-Dinitrotoluene
Concen: 7.306 ng
RT: 14.840 min Scan# 1966
Delta R.T. 0.422 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion:165 Resp: 13306
Ion Ratio Lower Upper
165 100
63 0.0 26.9 40.3#
89 0.0 35.6 53.4#

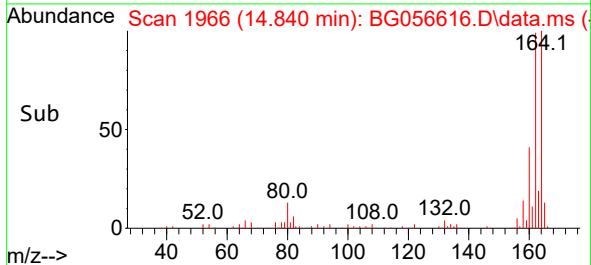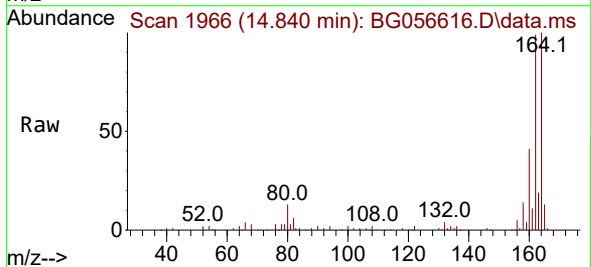



#57

2,4-Dinitrotoluene

Concen: 5.187 ng

RT: 14.840 min Scan# 1966

Delta R.T. -0.365 min

Lab File: BG056616.D


Acq: 10 Feb 2023 22:07

Instrument :

BNA_G

ClientSampleId :

COMP-1-BORING-1-0-7

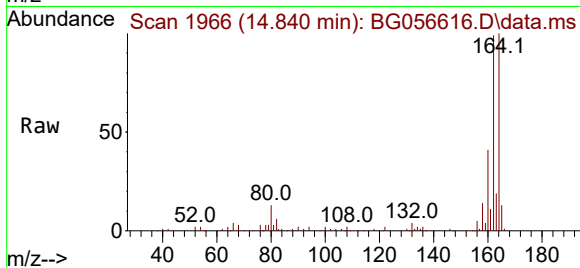

Tgt Ion:165 Resp: 13306




Ion Ratio Lower Upper

165 100

63 0.0 20.6 31.0#

89 0.0 43.1 64.7#

182 0.0 2.4 3.6#

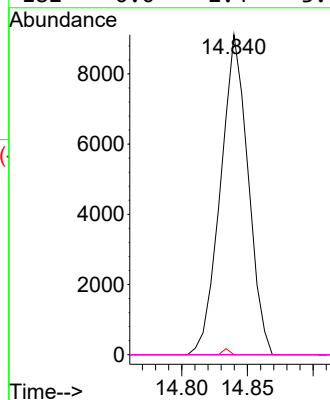

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.578 min Scan# 2432

Delta R.T. -0.007 min

Lab File: BG056616.D

Acq: 10 Feb 2023 22:07




Tgt Ion:188 Resp: 232539


Ion Ratio Lower Upper

188 100

94 5.1 4.1 6.1

80 6.5 5.0 7.4


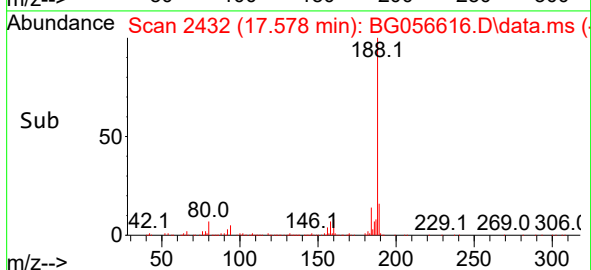
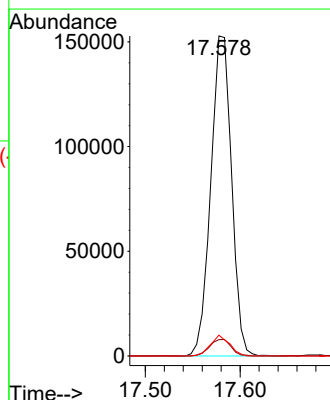
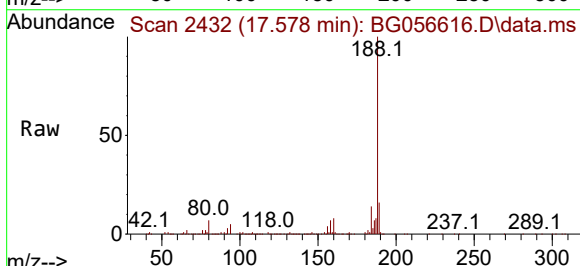




#67
4-Bromophenyl-phenylether
Concen: 4.770 ng
RT: 16.326 min Scan# 211
Delta R.T. -0.430 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07




Instrument :
BNA_G
ClientSampleId :
COMP-1-BORING-1-0-7


Tgt Ion:248 Resp: 14200
Ion Ratio Lower Upper
248 100
250 185.1 77.6 116.4#
141 387.8 39.0 58.4#

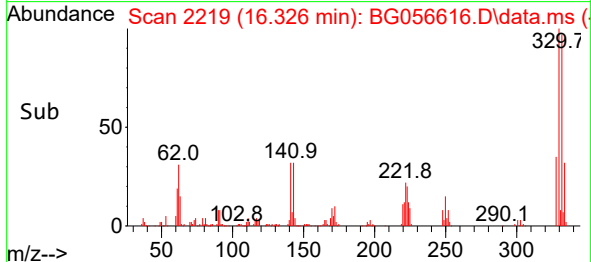

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.855 min Scan# 3160
Delta R.T. -0.007 min
Lab File: BG056616.D
Acq: 10 Feb 2023 22:07

Tgt Ion:240 Resp: 214564
Ion Ratio Lower Upper
240 100
120 4.5 3.8 5.8
236 25.8 20.2 30.2


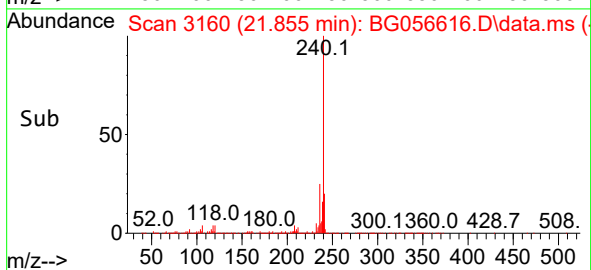

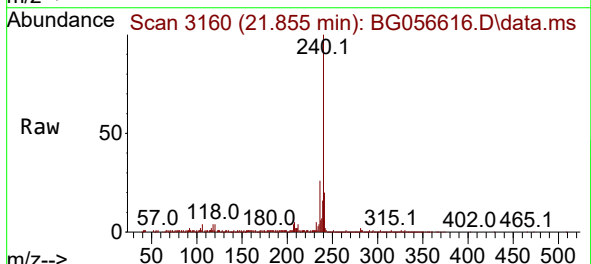




#79
 Terphenyl-d14
 Concen: 86.311 ng
 RT: 20.157 min Scan# 21
 Delta R.T. -0.001 min
 Lab File: BG056616.D
 Acq: 10 Feb 2023 22:07




Instrument :
 BNA_G
 ClientSampleId :
 COMP-1-BORING-1-0-7


Tgt Ion:244 Resp: 1054412
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.5 8.3
 122 5.1 4.4 6.6

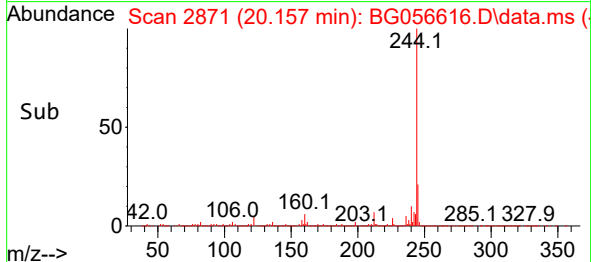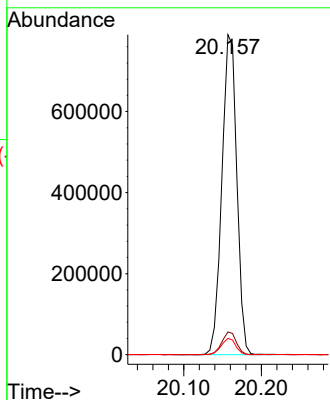

#85
 Di-n-octyl phthalate
 Concen: 8.176 ng
 RT: 23.024 min Scan# 3359
 Delta R.T. 0.075 min
 Lab File: BG056616.D
 Acq: 10 Feb 2023 22:07

Tgt Ion:149 Resp: 90977
 Ion Ratio Lower Upper
 149 100
 167 49.8 1.4 2.0#
 43 9.9 2.7 4.1#

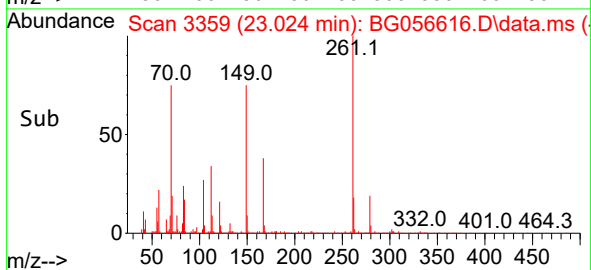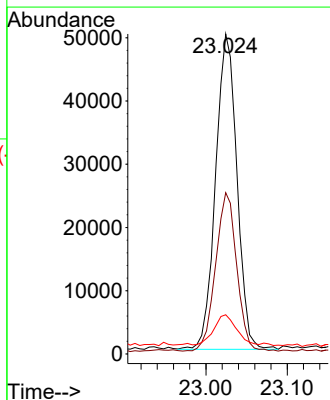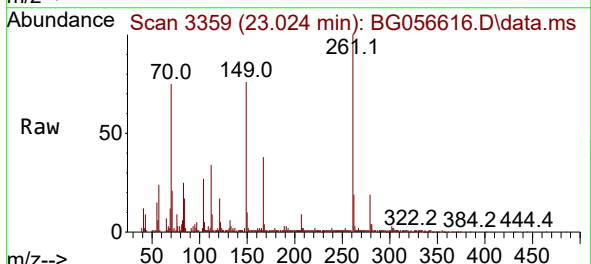

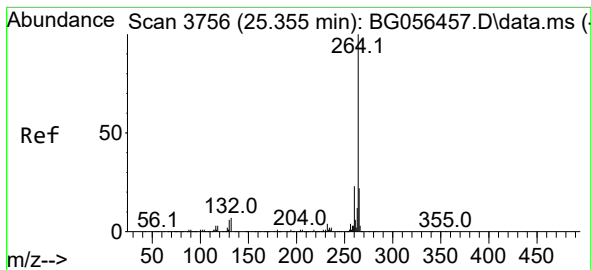

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.239 min Scan# 31

Delta R.T. 0.005 min

Lab File: BG056616.D


Acq: 10 Feb 2023 22:07

Instrument :

BNA_G

ClientSampleId :

COMP-1-BORING-1-0-7

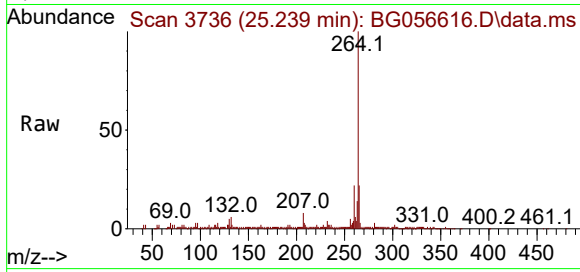

Tgt Ion:264 Resp: 238030

Ion Ratio Lower Upper

264 100

260 22.3 18.2 27.4

265 21.7 18.1 27.1

