
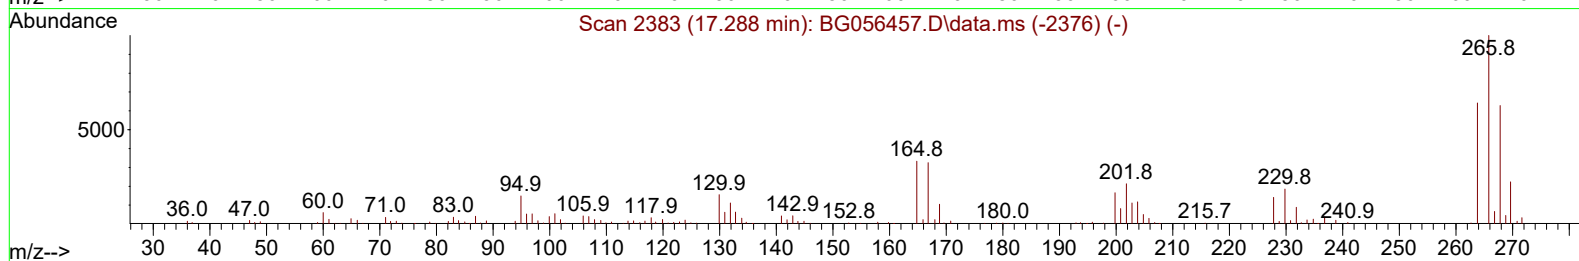
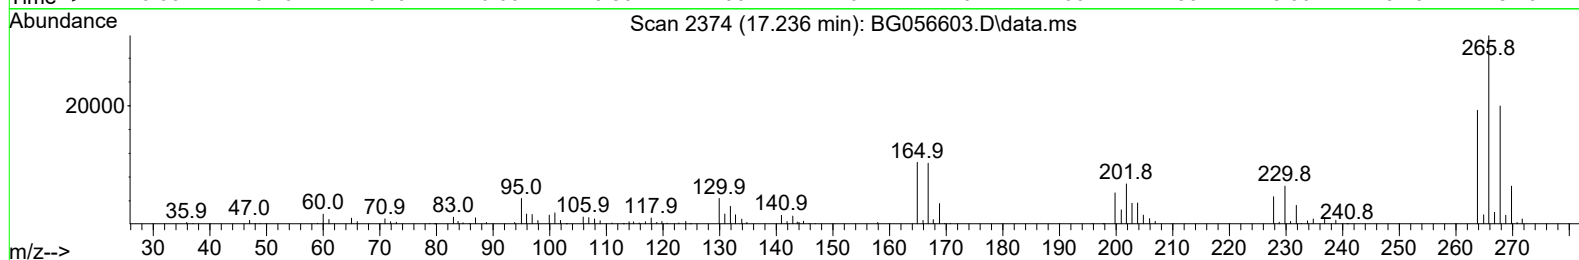


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056603.D
Acq On : 10 Feb 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:01:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

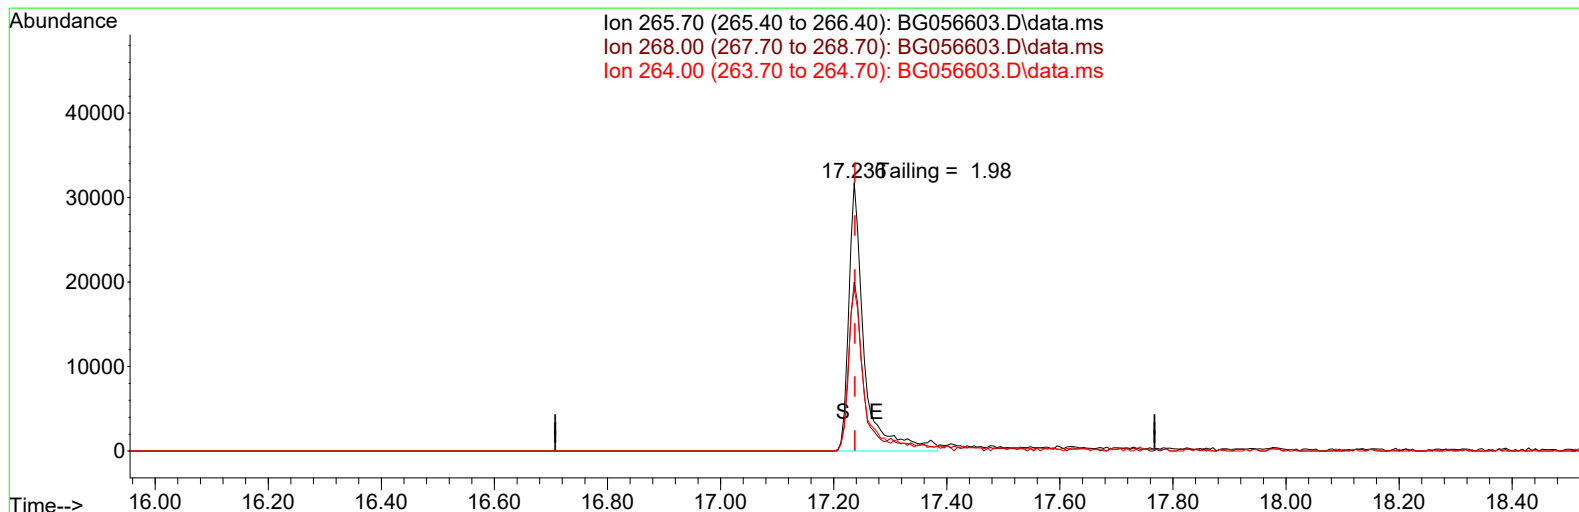

TIC: BG056603.D\data.ms

(70) Pentachlorophenol (C)




17.236min (-0.002) 16296.74 ng

response 58976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.81
264.00	64.20	60.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056603.D
Acq On : 10 Feb 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:01:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

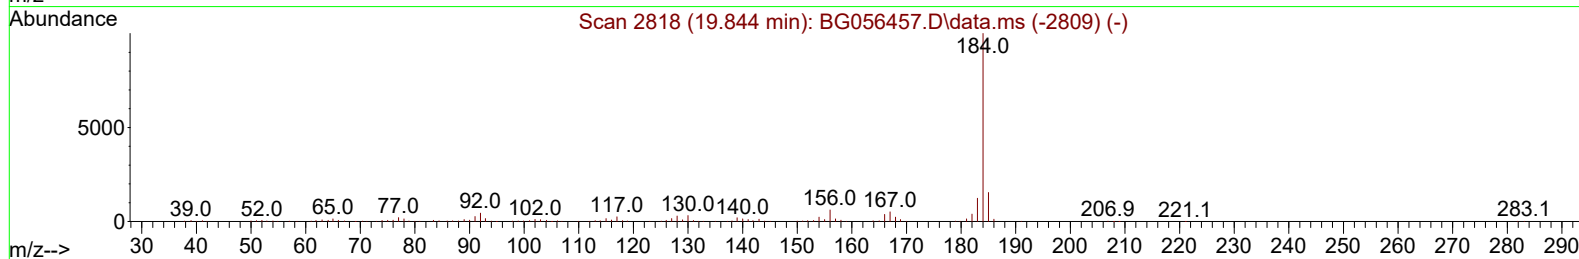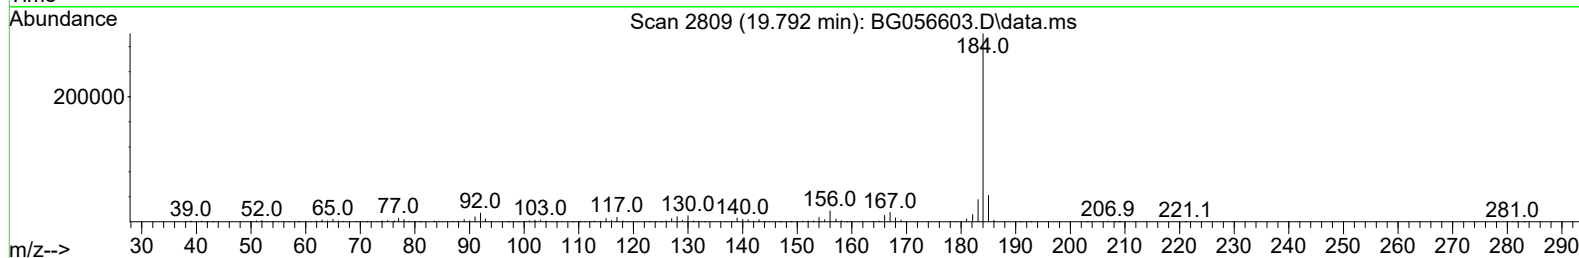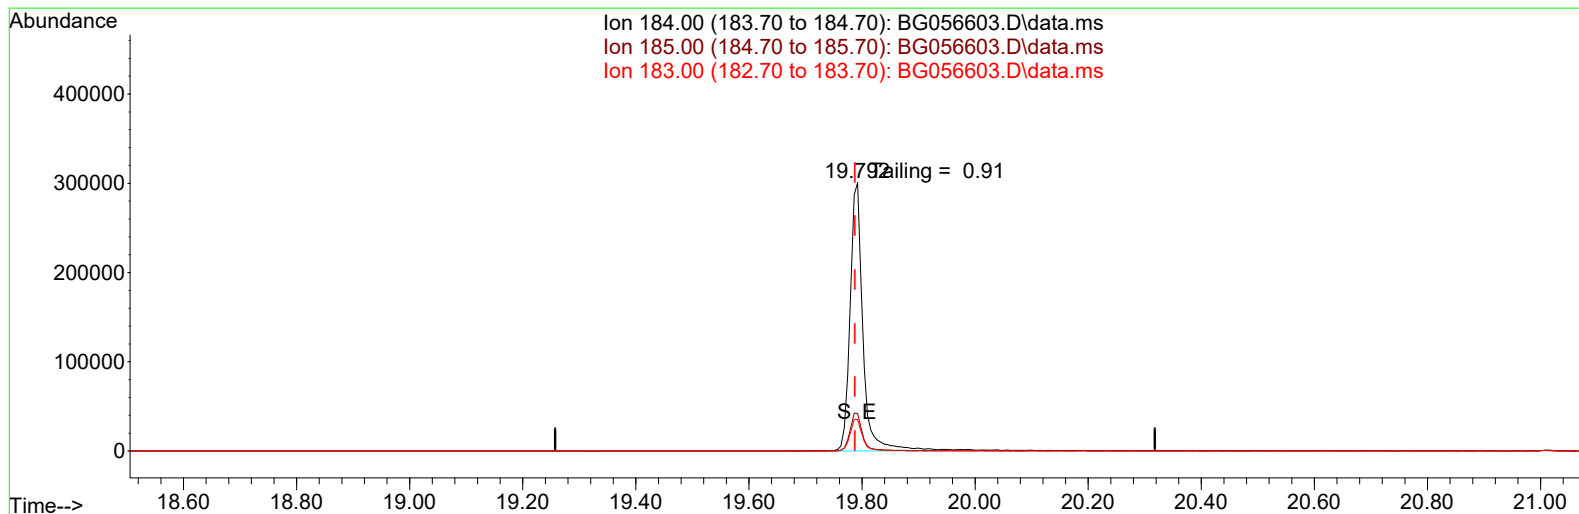

TIC: BG056603.D\data.ms

(77) Benzidine**19.792min (+ 0.004) 294973.27 ng****response 478940**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.04
183.00	12.30	11.78
0.00	0.00	0.00