

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
 Data File : BG056617.D
 Acq On : 10 Feb 2023 22:48
 Operator : CG/JU
 Sample : 01328-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-5-BORING-2-0-7

Quant Time: Feb 10 23:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 10 22:46:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.214	152	40347	20.000	ng	0.00
21) Naphthalene-d8	11.046	136	148265	20.000	ng	0.00
39) Acenaphthene-d10	14.841	164	106464	20.000	ng	0.00
64) Phenanthrene-d10	17.579	188	234998	20.000	ng	0.00
76) Chrysene-d12	21.856	240	211058	20.000	ng	0.00
86) Perylene-d12	25.235	264	223241	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.740	112	208825	95.212	ng	0.01
7) Phenol-d6	7.373	99	286735	88.234	ng	0.00
23) Nitrobenzene-d5	9.395	82	151123	57.880	ng	0.00
42) 2,4,6-Tribromophenol	16.328	330	113685	80.321	ng	0.00
45) 2-Fluorobiphenyl	13.466	172	450200	58.627	ng	0.00
79) Terphenyl-d14	20.158	244	626978	52.175	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056617.D
Acq On : 10 Feb 2023 22:48
Operator : CG/JU
Sample : 01328-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-5-BORING-2-0-7


Quant Time: Feb 10 23:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

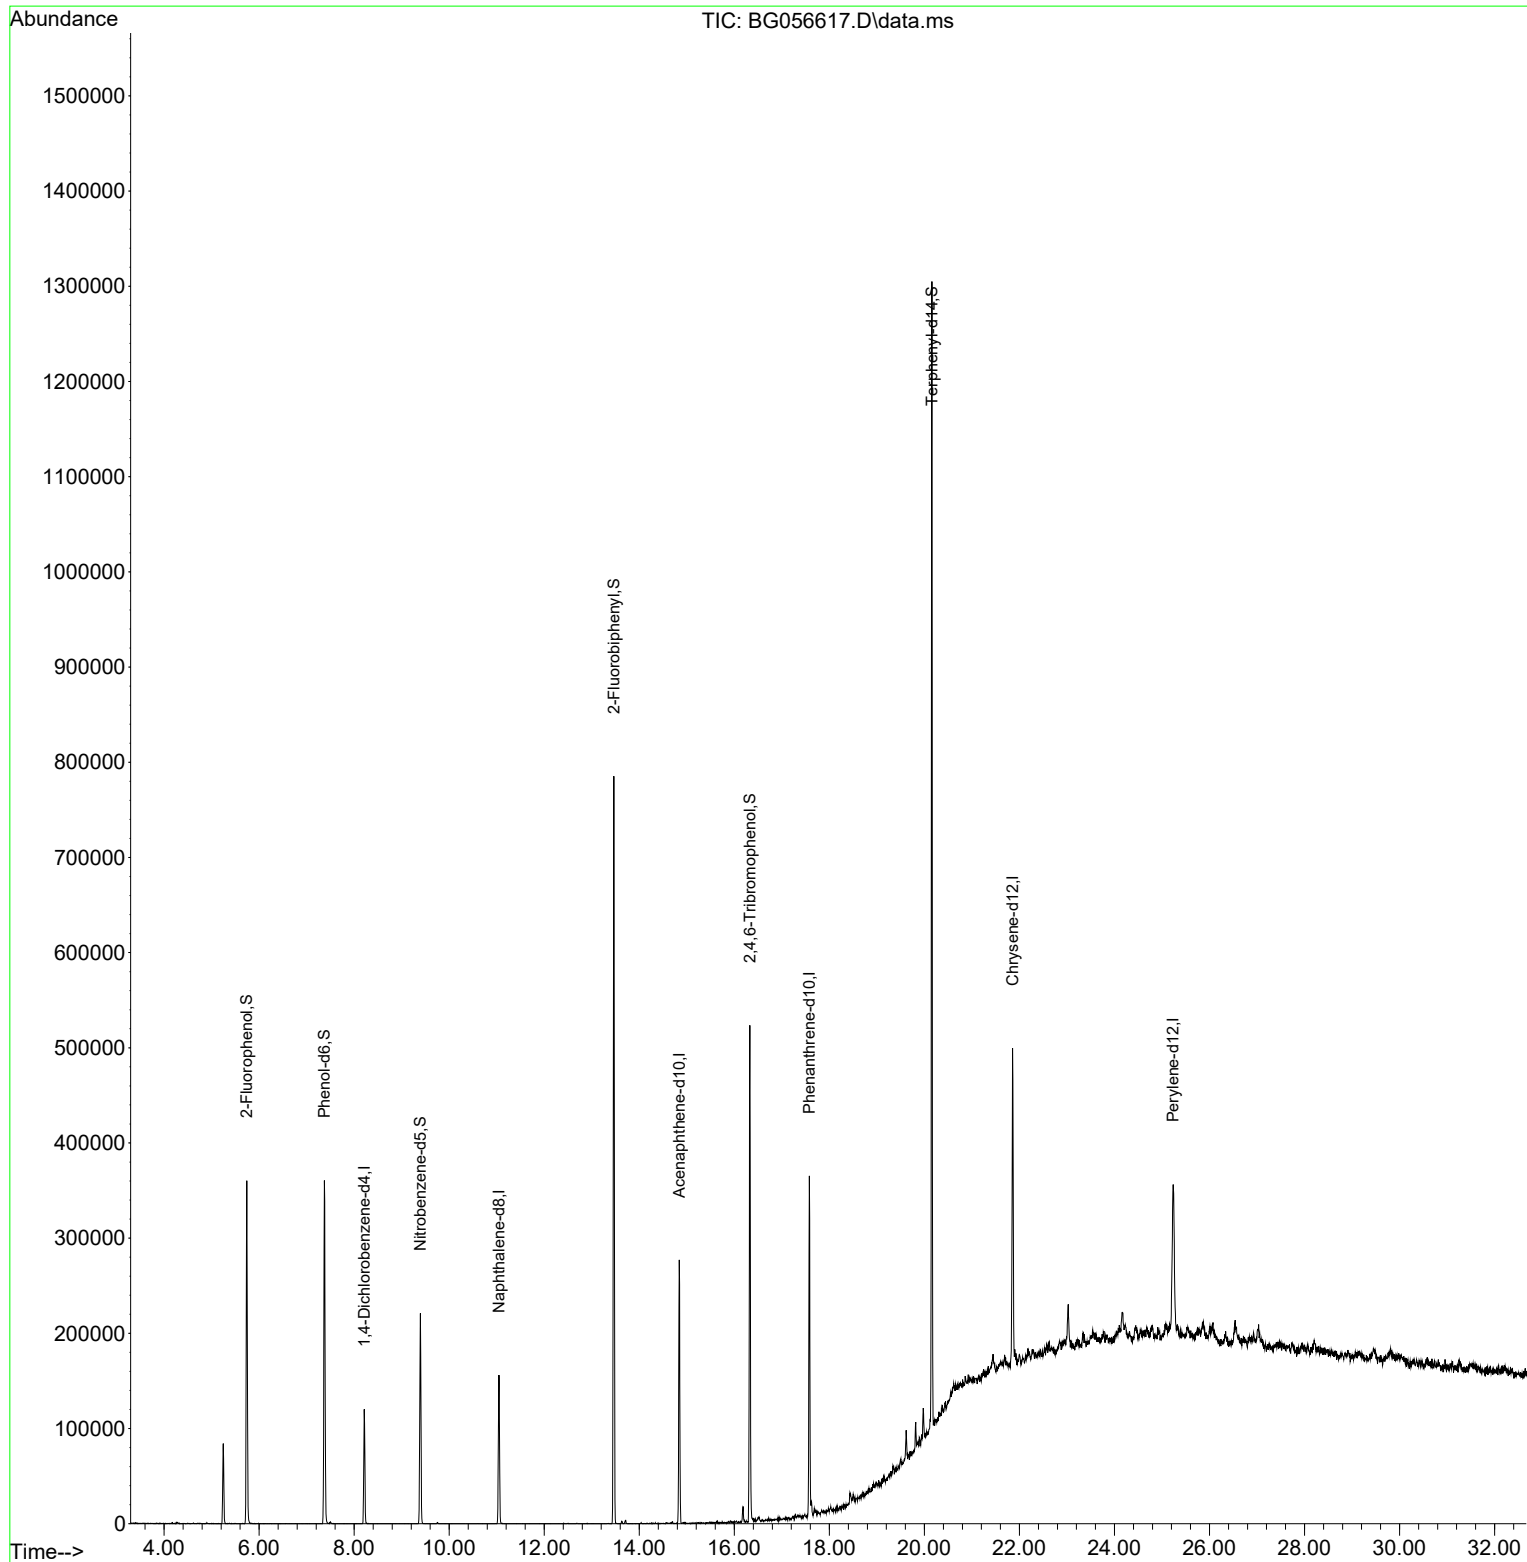






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.214 min Scan# 81
Delta R.T. 0.007 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48


Instrument :
BNA_G
ClientSampleId :
COMP-5-BORING-2-0-7





Tgt Ion:152 Resp: 40347
Ion Ratio Lower Upper
152 100
150 143.0 120.2 180.4
115 49.6 36.3 54.5

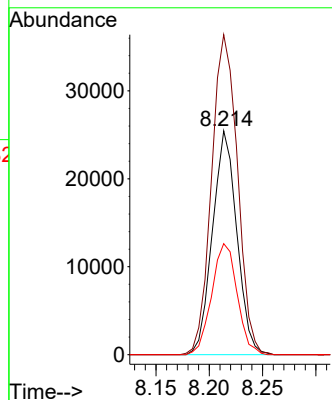


#5
2-Fluorophenol
Concen: 95.212 ng
RT: 5.740 min Scan# 417
Delta R.T. 0.012 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48

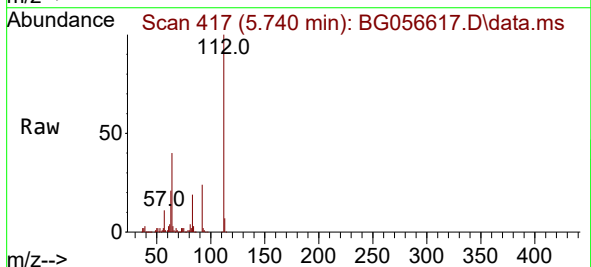

Tgt Ion:112 Resp: 208825
Ion Ratio Lower Upper
112 100
64 39.7 31.9 47.9
63 21.5 17.4 26.0



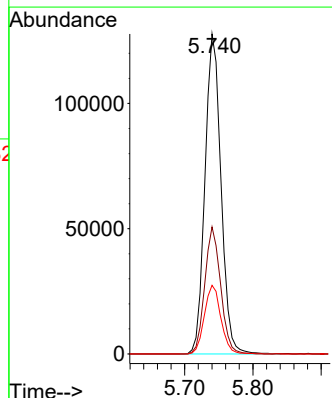





#7
Phenol-d6
Concen: 88.234 ng
RT: 7.373 min Scan# 61
Delta R.T. 0.006 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48




Instrument :
BNA_G
ClientSampleId :
COMP-5-BORING-2-0-7


Tgt Ion: 99 Resp: 286735
Ion Ratio Lower Upper
99 100
42 8.3 6.6 10.0
71 29.5 23.4 35.0

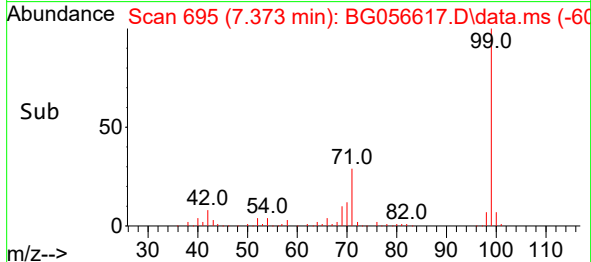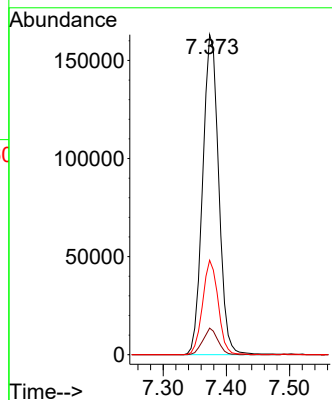

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.046 min Scan# 1320
Delta R.T. 0.000 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48

Tgt Ion: 136 Resp: 148265
Ion Ratio Lower Upper
136 100
137 11.9 9.4 14.0
54 2.8 2.2 3.4
68 4.1 3.6 5.4

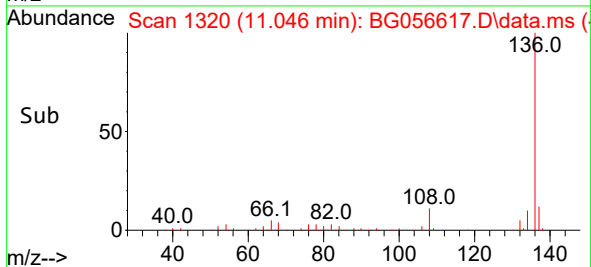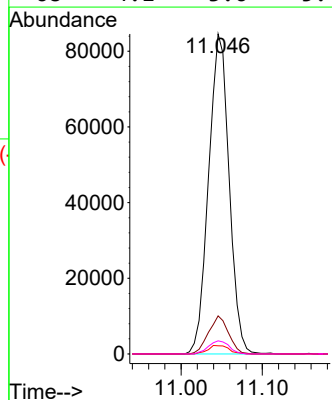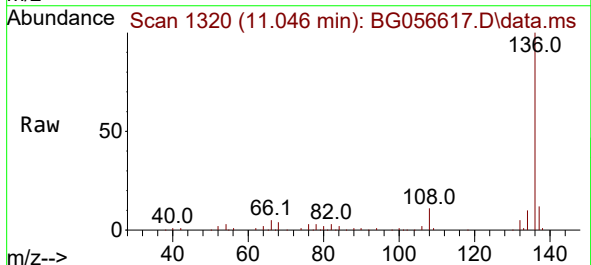



#23

Nitrobenzene-d5

Concen: 57.880 ng

RT: 9.395 min Scan# 1039

Delta R.T. 0.006 min

Lab File: BG056617.D

Acq: 10 Feb 2023 22:48

Instrument :

BNA_G

ClientSampleId :

COMP-5-BORING-2-0-7





Tgt Ion: 82 Resp: 151123

Ion Ratio Lower Upper

82 100

128 49.8 39.4 59.2

54 26.8 21.4 32.2

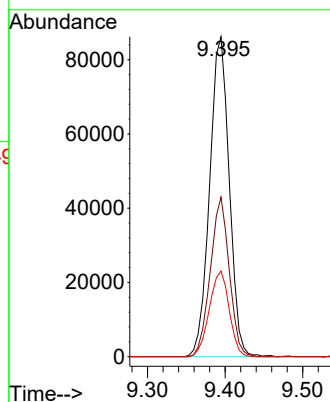

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.841 min Scan# 1966

Delta R.T. 0.000 min

Lab File: BG056617.D

Acq: 10 Feb 2023 22:48




Tgt Ion:164 Resp: 106464


Ion Ratio Lower Upper

164 100

162 105.4 79.6 119.4

160 42.8 34.9 52.3


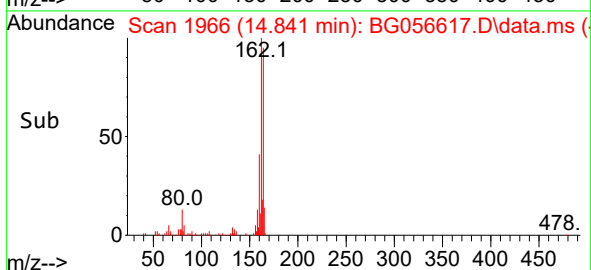
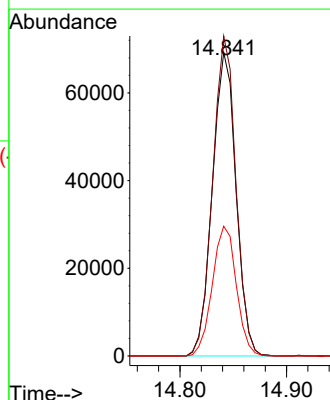





#42
2,4,6-Tribromophenol
Concen: 80.321 ng
RT: 16.328 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48




Instrument :
BNA_G
ClientSampleId :
COMP-5-BORING-2-0-7


Tgt Ion:330 Resp: 113685
Ion Ratio Lower Upper
330 100
332 96.5 79.0 118.6
141 29.4 24.2 36.4

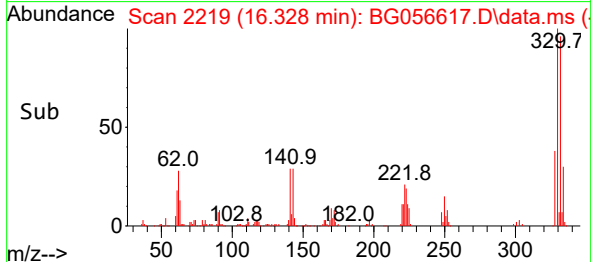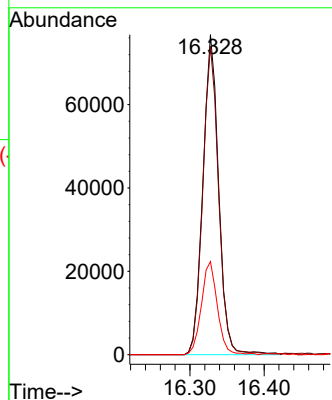

#45
2-Fluorobiphenyl
Concen: 58.627 ng
RT: 13.466 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48

Tgt Ion:172 Resp: 450200
Ion Ratio Lower Upper
172 100
171 35.9 29.5 44.3
170 23.6 19.2 28.8


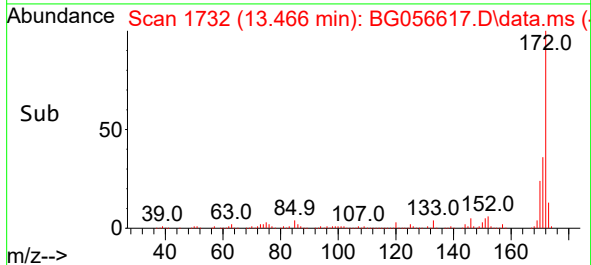
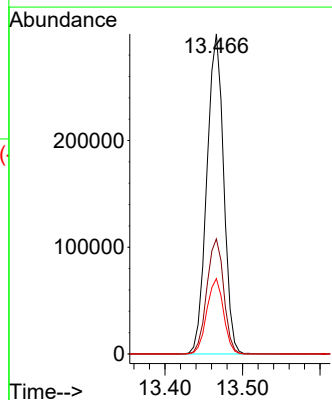
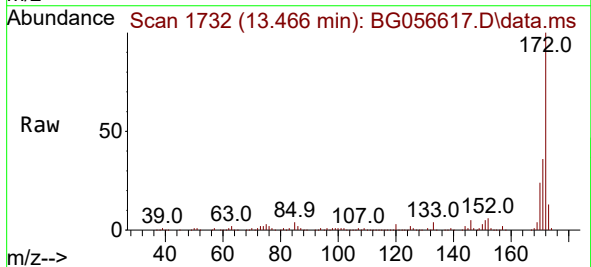




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.579 min Scan# 2443
Delta R.T. -0.005 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48




Instrument :
BNA_G
ClientSampleId :
COMP-5-BORING-2-0-7


Tgt Ion:188 Resp: 234998
Ion Ratio Lower Upper
188 100
94 5.7 4.1 6.1
80 5.0 5.0 7.4

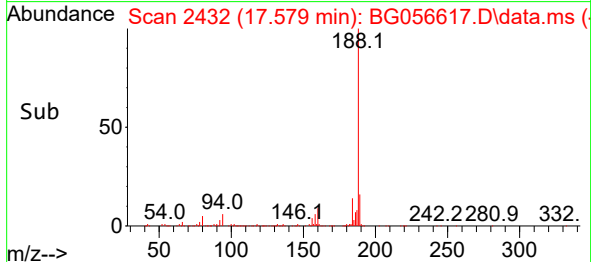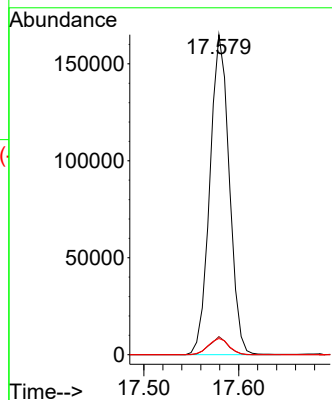

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.856 min Scan# 3160
Delta R.T. -0.005 min
Lab File: BG056617.D
Acq: 10 Feb 2023 22:48

Tgt Ion:240 Resp: 211058
Ion Ratio Lower Upper
240 100
120 4.5 3.8 5.8
236 25.7 20.2 30.2


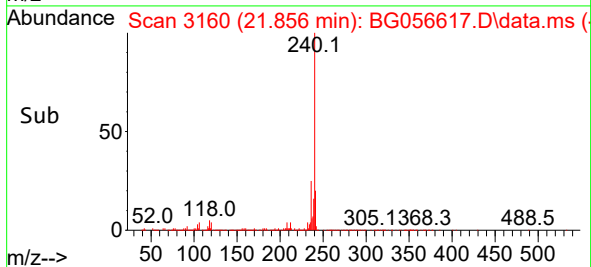
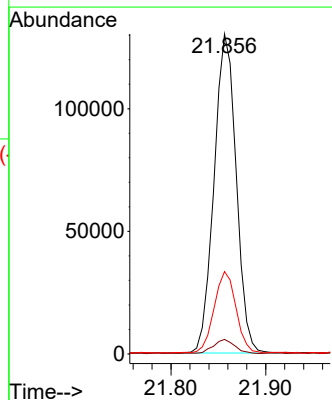
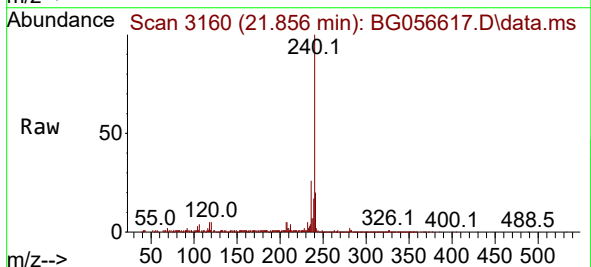




#79
 Terphenyl-d14
 Concen: 52.175 ng
 RT: 20.158 min Scan# 2
 Delta R.T. 0.000 min
 Lab File: BG056617.D
 Acq: 10 Feb 2023 22:48

Instrument :
 BNA_G
 ClientSampleId :
 COMP-5-BORING-2-0-7

Tgt Ion:244 Resp: 626978
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.5 8.3
 122 4.9 4.4 6.6

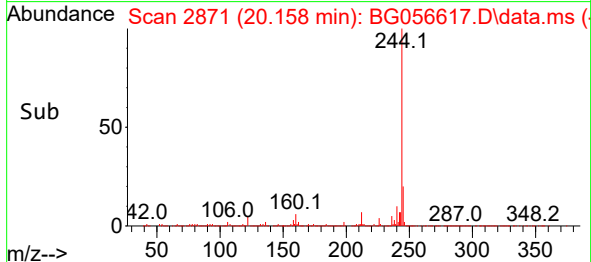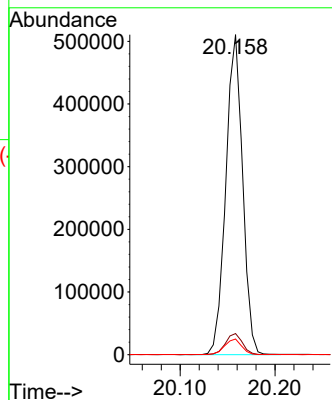

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.235 min Scan# 3735
 Delta R.T. 0.000 min
 Lab File: BG056617.D
 Acq: 10 Feb 2023 22:48

Tgt Ion:264 Resp: 223241
 Ion Ratio Lower Upper
 264 100
 260 24.4 18.2 27.4
 265 22.5 18.1 27.1

