


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056603.D
Acq On : 10 Feb 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 10 22:46:08 2023

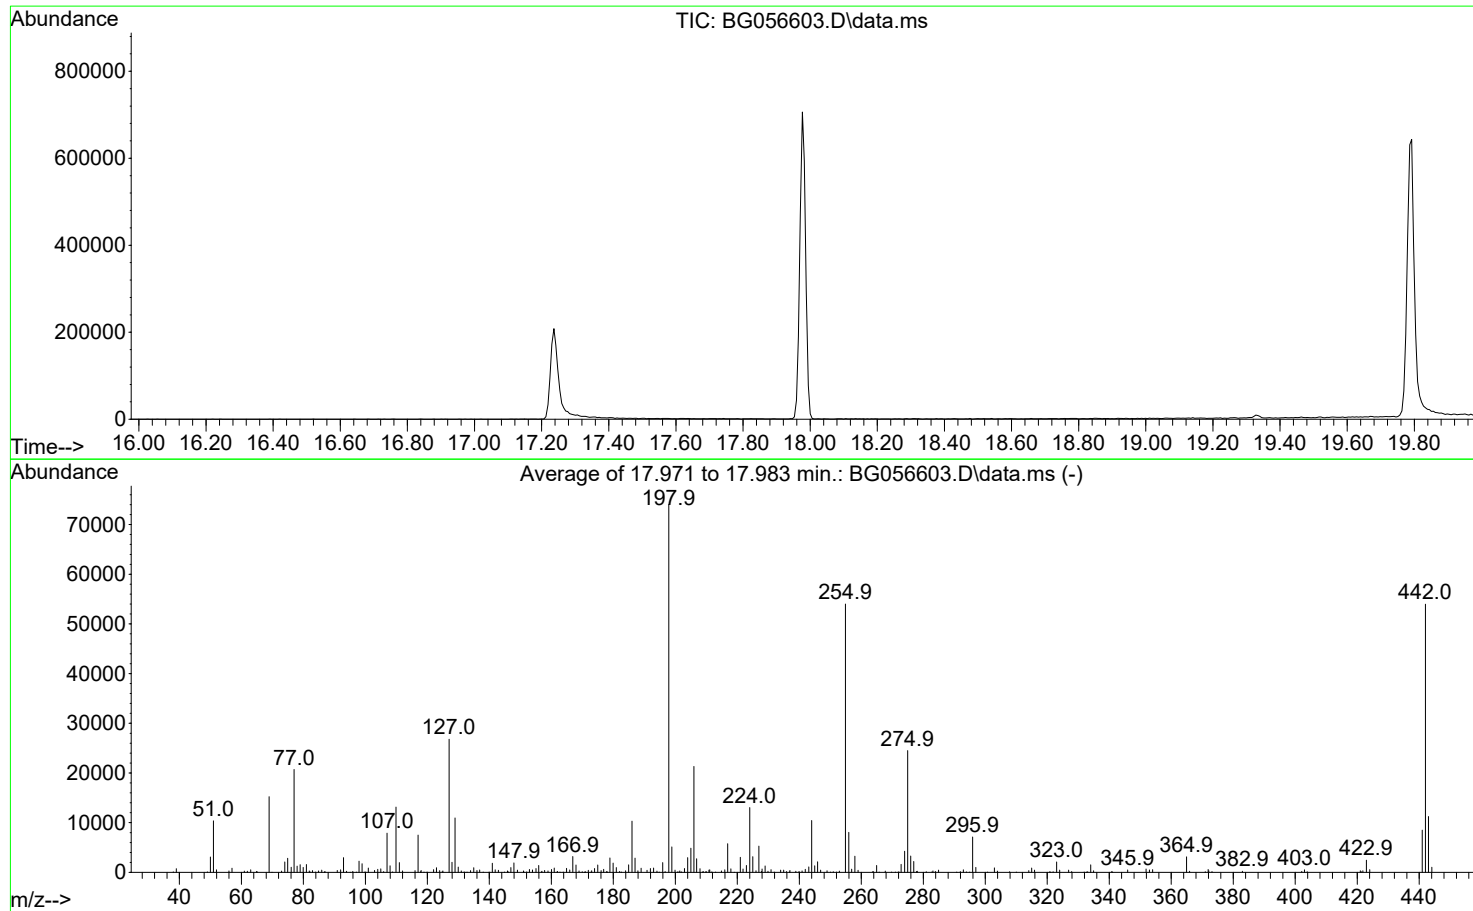

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.0	10374	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.6	15247	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	36.2	26803	PASS
197	198	0.00	2	0.2	174	PASS
198	198	100	100	100.0	74035	PASS
199	198	5	9	6.9	5136	PASS
275	198	10	60	33.1	24512	PASS
365	198	1	100	4.2	3126	PASS
441	198	0.01	100	11.5	8489	PASS
442	442	50	100	100.0	53987	PASS
443	442	15	24	20.8	11224	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/10/2023	BNA_G	BG056603.D
Compound Name	Response	Retention Time
DDT	259955	21.014
DDD	7723	20.568
DDE	763	20.062
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8486	268441	3.16

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056603.D
Acq On : 10 Feb 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 11 03:01:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

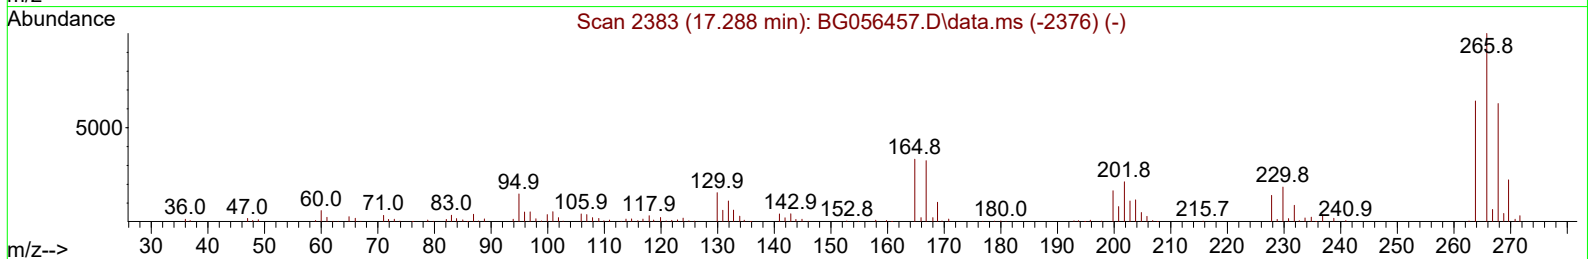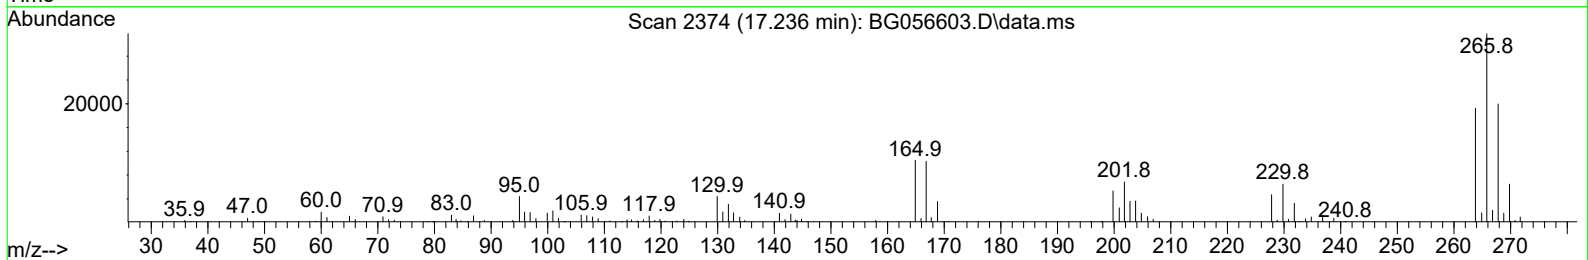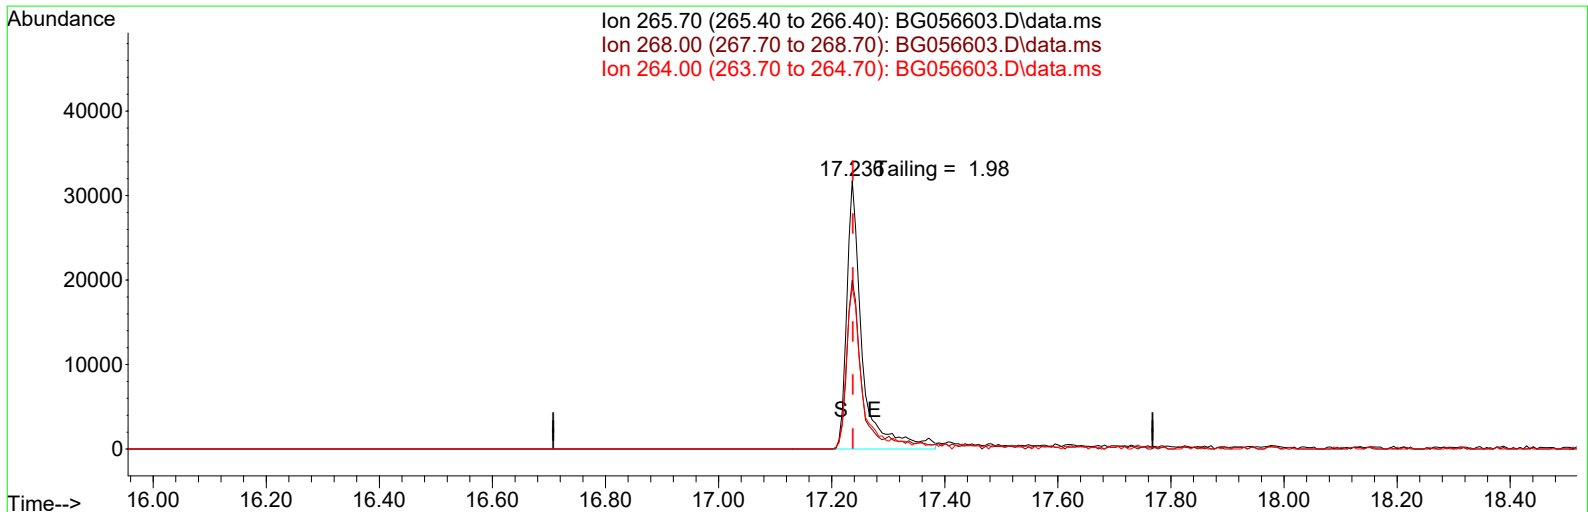

TIC: BG056603.D\data.ms

(70) Pentachlorophenol (C)

17.236min (-0.002) 16296.74 ng




response 58976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.81
264.00	64.20	60.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021023\
Data File : BG056603.D
Acq On : 10 Feb 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 11 03:01:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

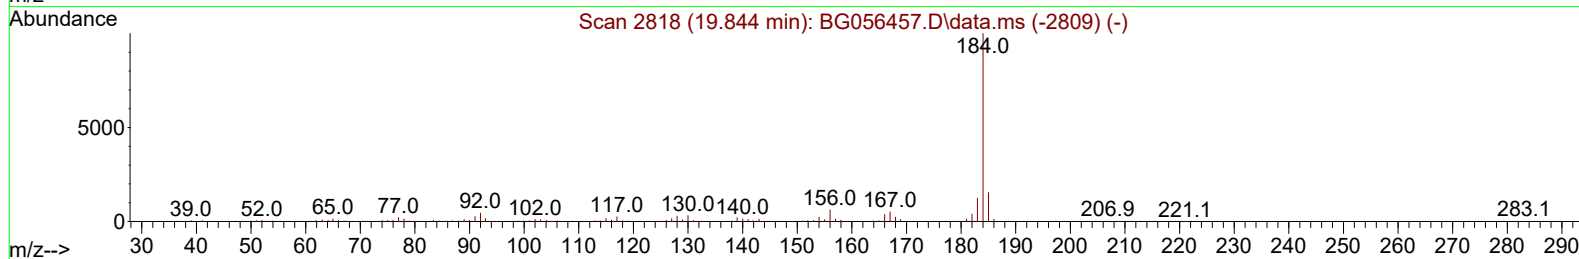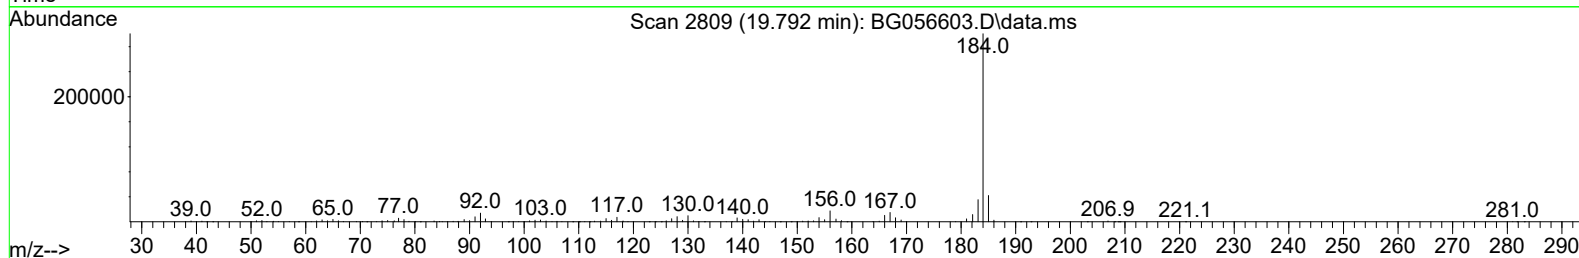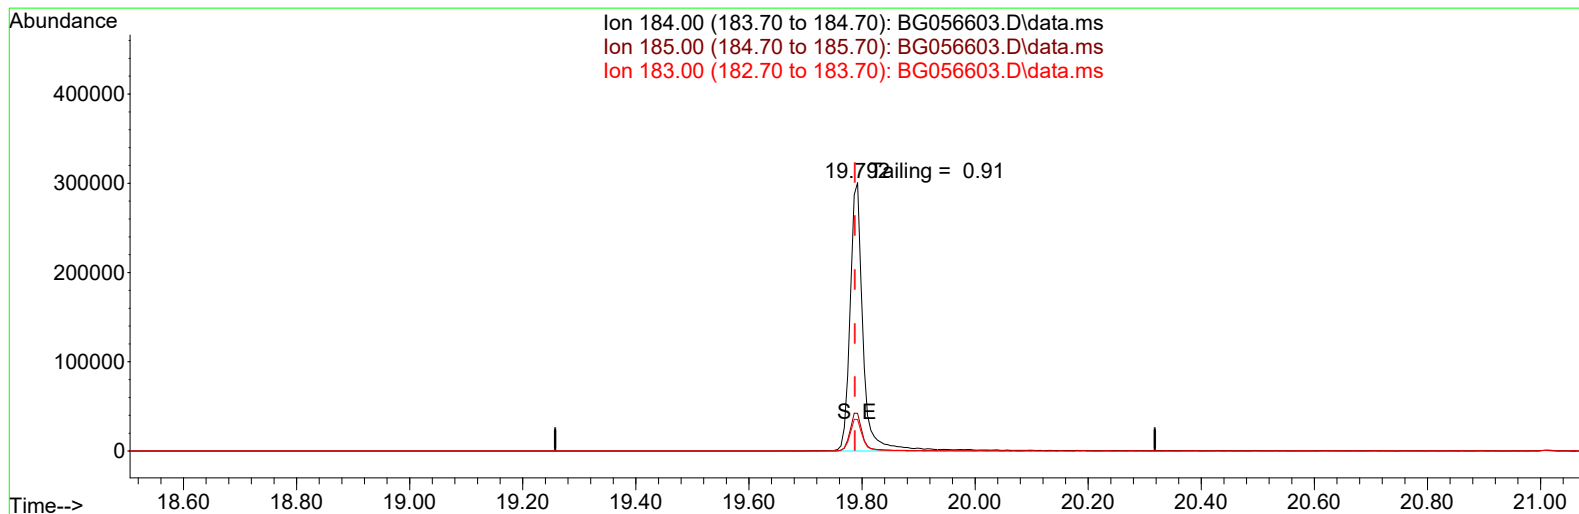

TIC: BG056603.D\data.ms

(77) Benzidine

19.792min (+ 0.004) 294973.27 ng

response 478940

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.04
183.00	12.30	11.78
0.00	0.00	0.00