


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\  
Data File : BG020849.D  
Acq On : 11 Feb 2016 10:12  
Operator : SJ/UM  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:42:30 2016  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 11 15:26:53 2016  
Response via : Initial Calibration

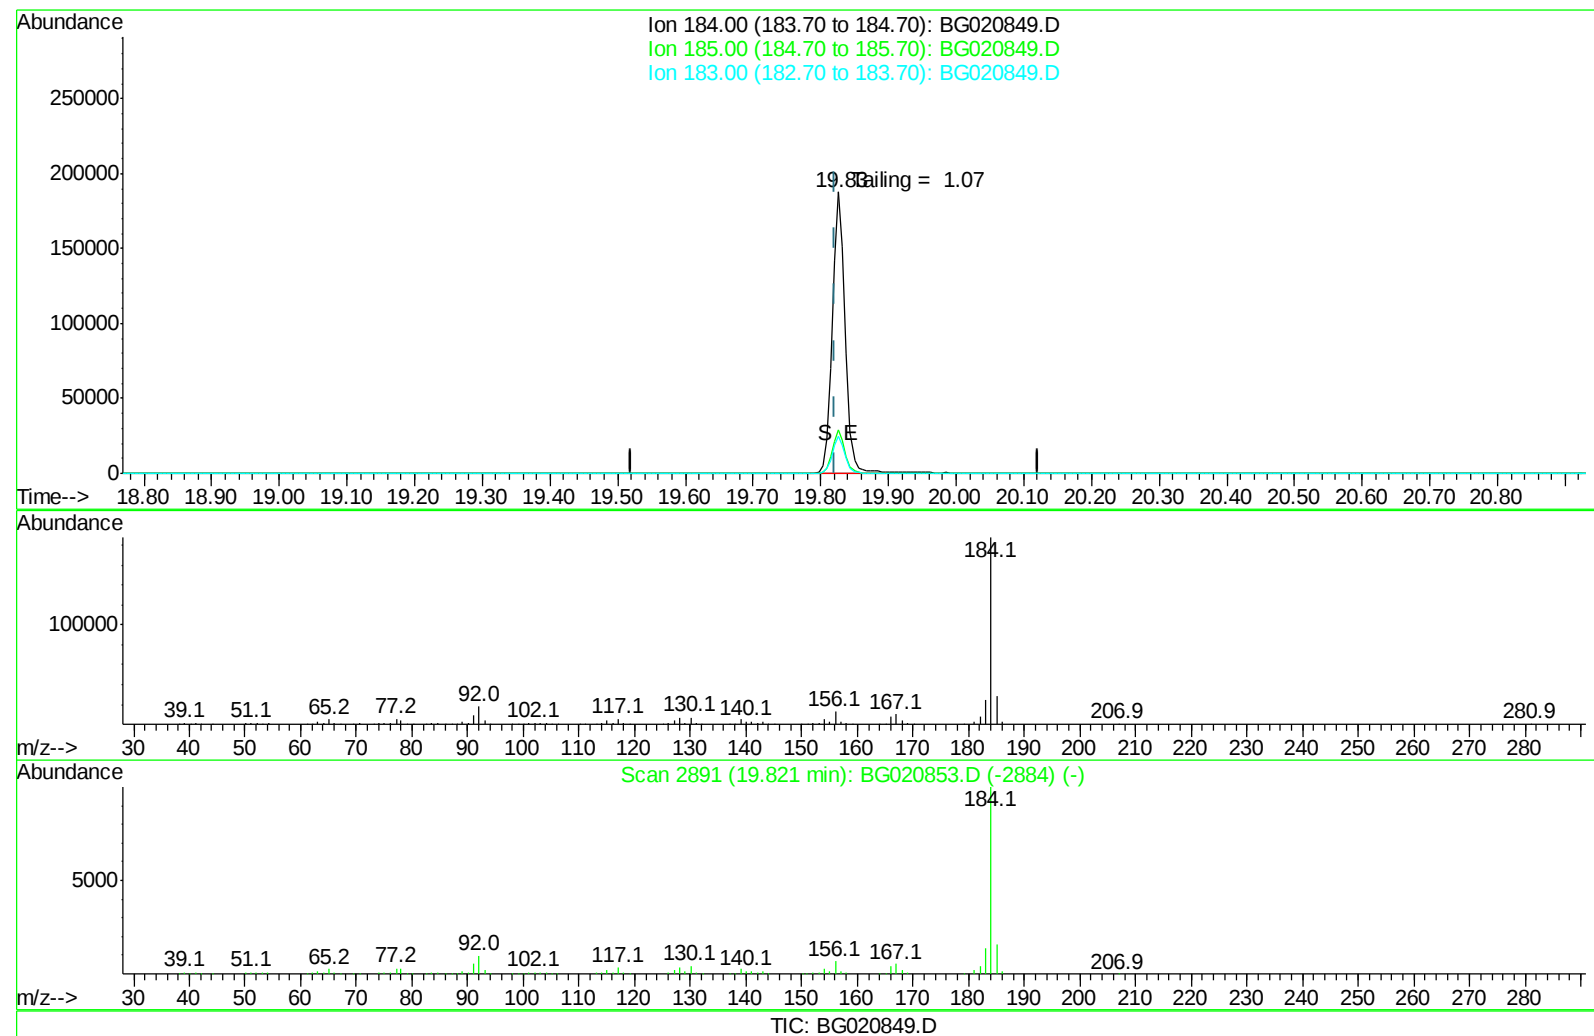

TIC: BG020849.D

(76) Benzidine




19.826min (+0.005) 0.00ng

response 252093

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 15.37 |
| 183.00 | 13.70 | 13.27 |
| 0.00   | 0.00  | 0.00  |

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\  
Data File : BG020849.D  
Acq On : 11 Feb 2016 10:12  
Operator : SJ/UM  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:42:30 2016  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 11 15:26:53 2016  
Response via : Initial Calibration

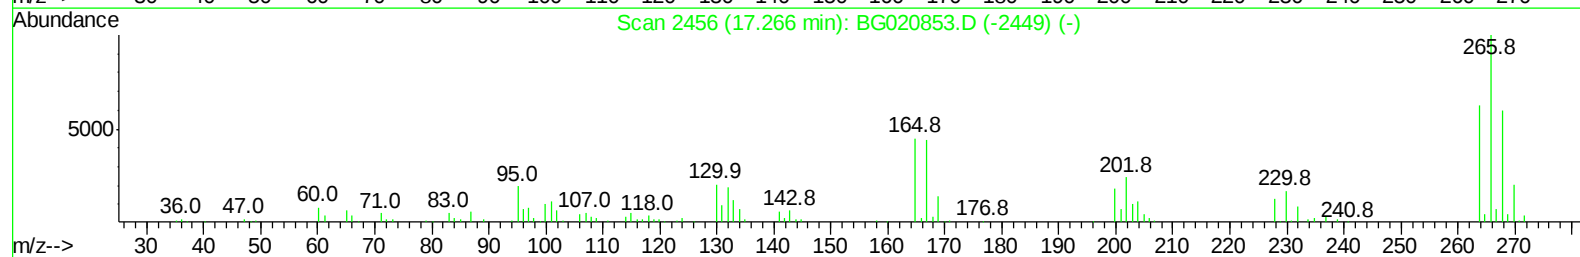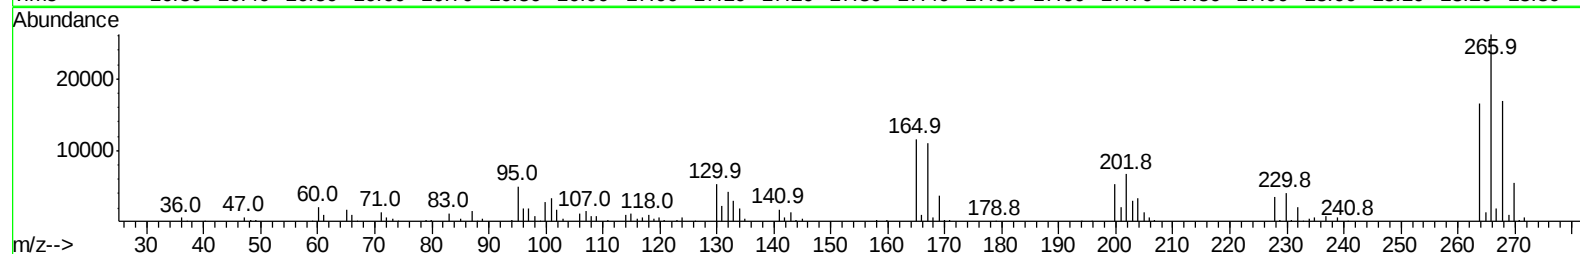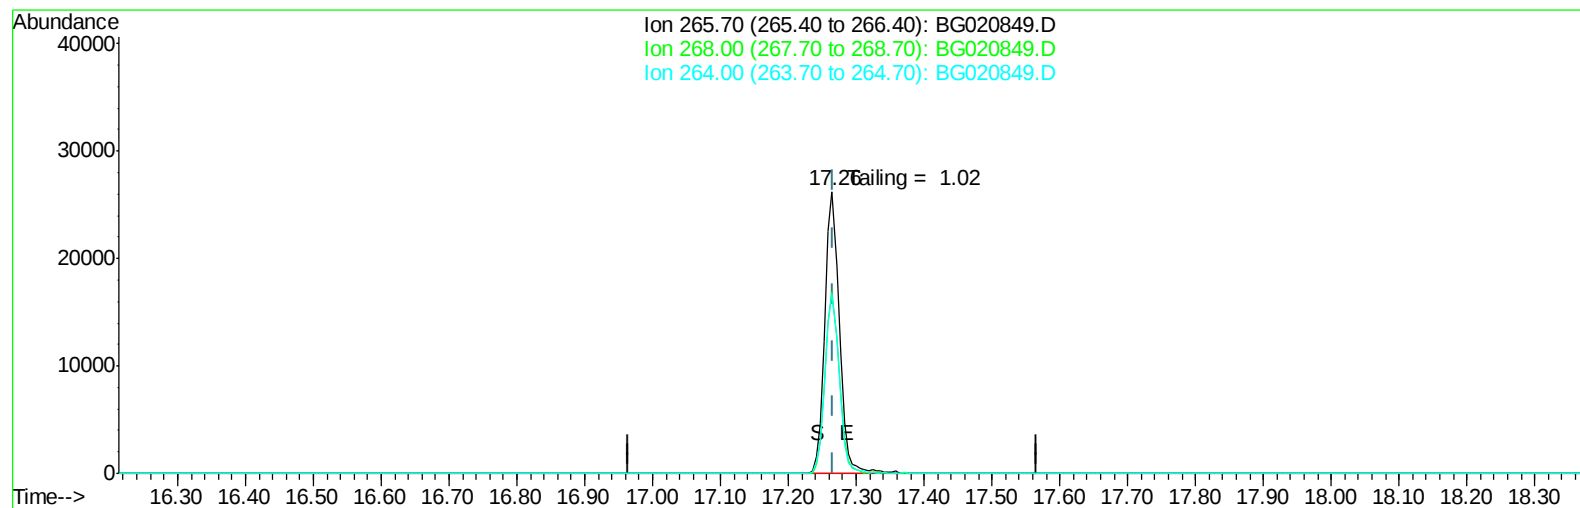

TIC: BG020849.D

(69) Pentachlorophenol (C)

17.265min (-0.001) 15276.80ng

response 38288

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 59.70 | 64.35 |
| 264.00 | 62.80 | 63.43 |
| 0.00   | 0.00  | 0.00  |