
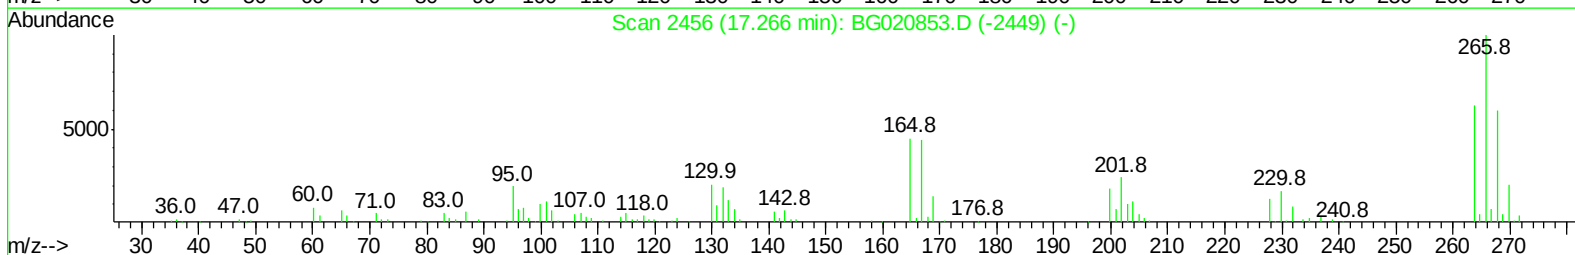
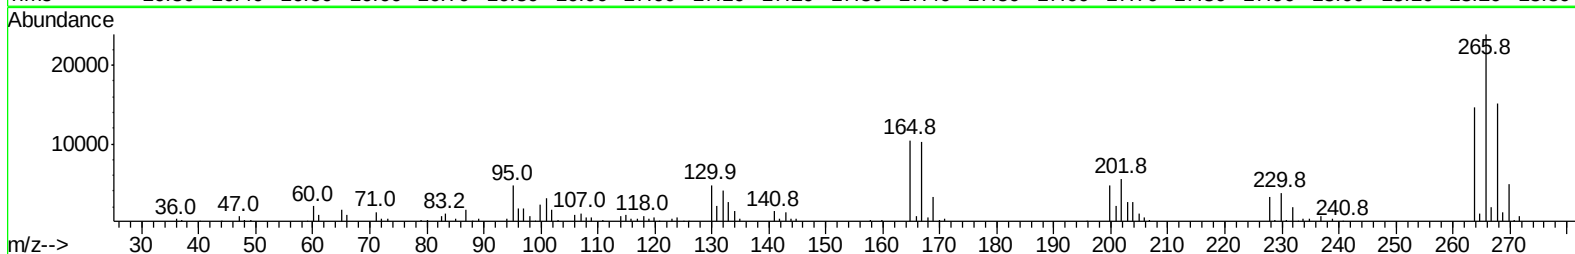


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\
Data File : BG020859.D
Acq On : 11 Feb 2016 16:51
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 18:05:45 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

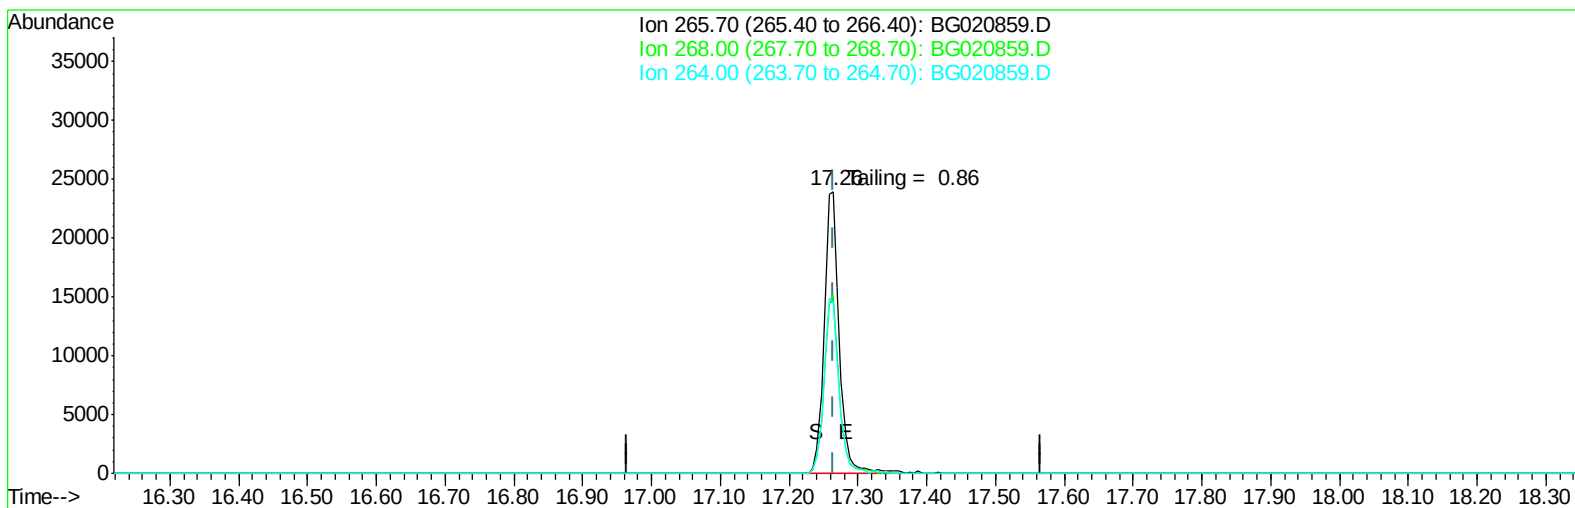

TIC: BG020859.D

(69) Pentachlorophenol (C)




17.264min (-0.002) 14902.99ng

response 36679

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	63.33
264.00	62.80	61.05
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\
 Data File : BG020859.D
 Acq On : 11 Feb 2016 16:51
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 18:05:45 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 11 15:26:53 2016
 Response via : Initial Calibration

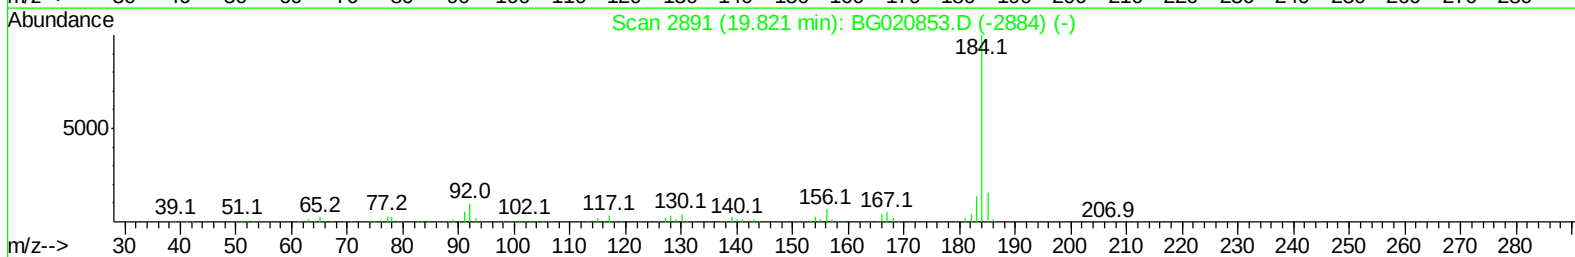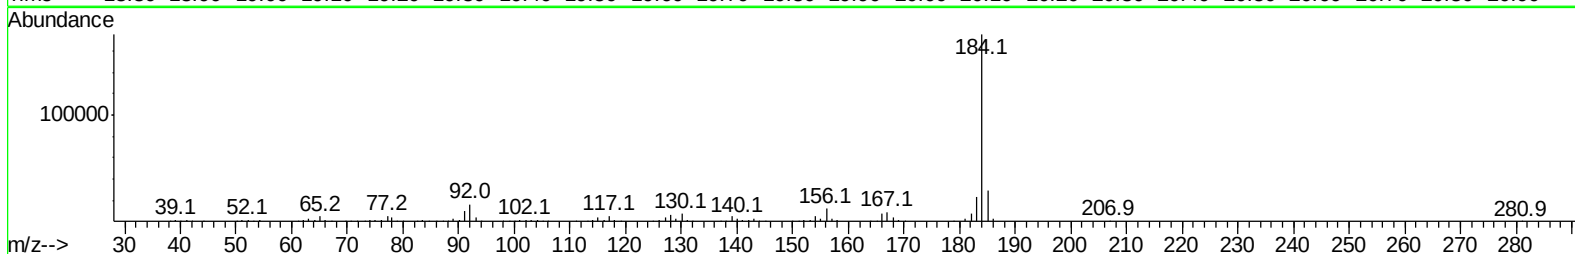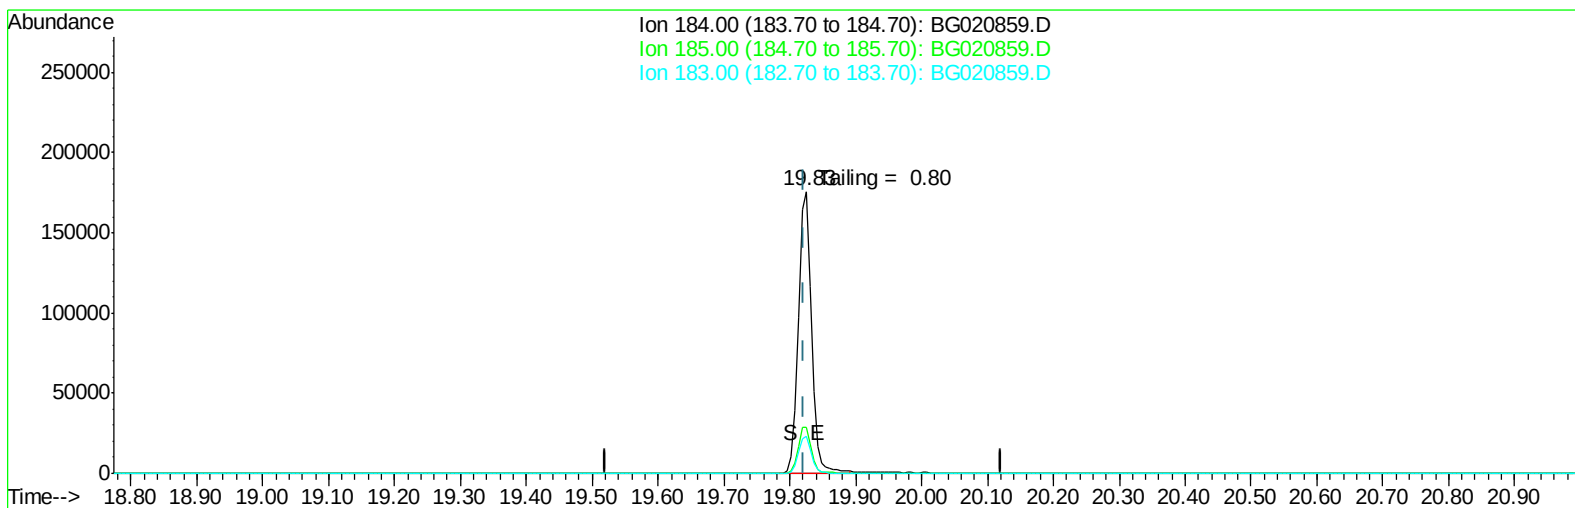

TIC: BG020859.D

(76) Benzidine

19.825min (+0.004) 0.00ng

response 249870

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.59
183.00	13.70	13.09
0.00	0.00	0.00