
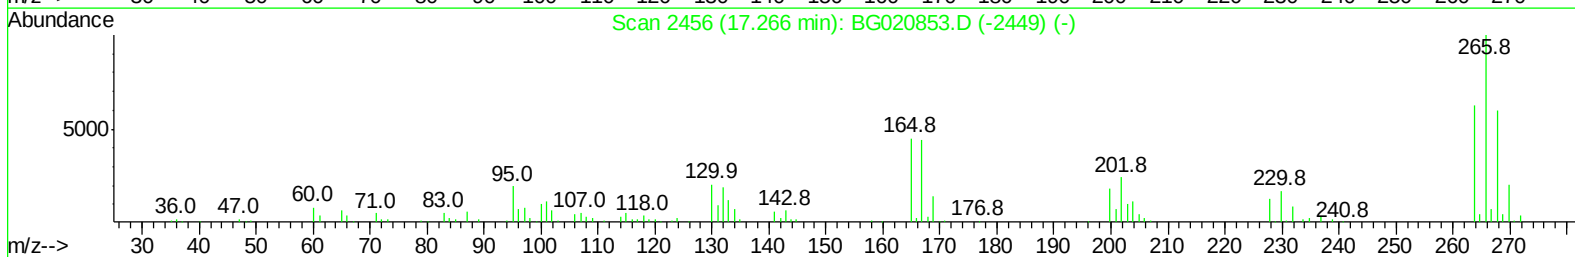
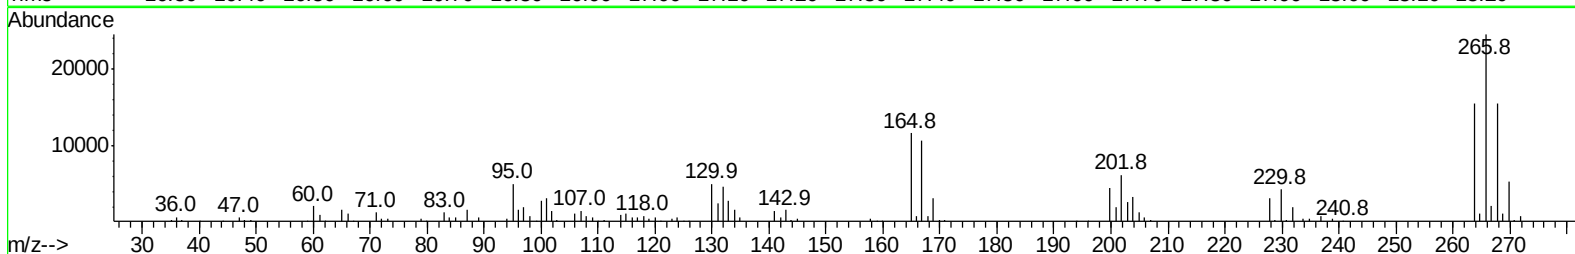


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\
Data File : BG020873.D
Acq On : 12 Feb 2016 1:59
Operator : SJ/UM
Sample : DFTPP
Misc : L00 20PPM
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:31:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

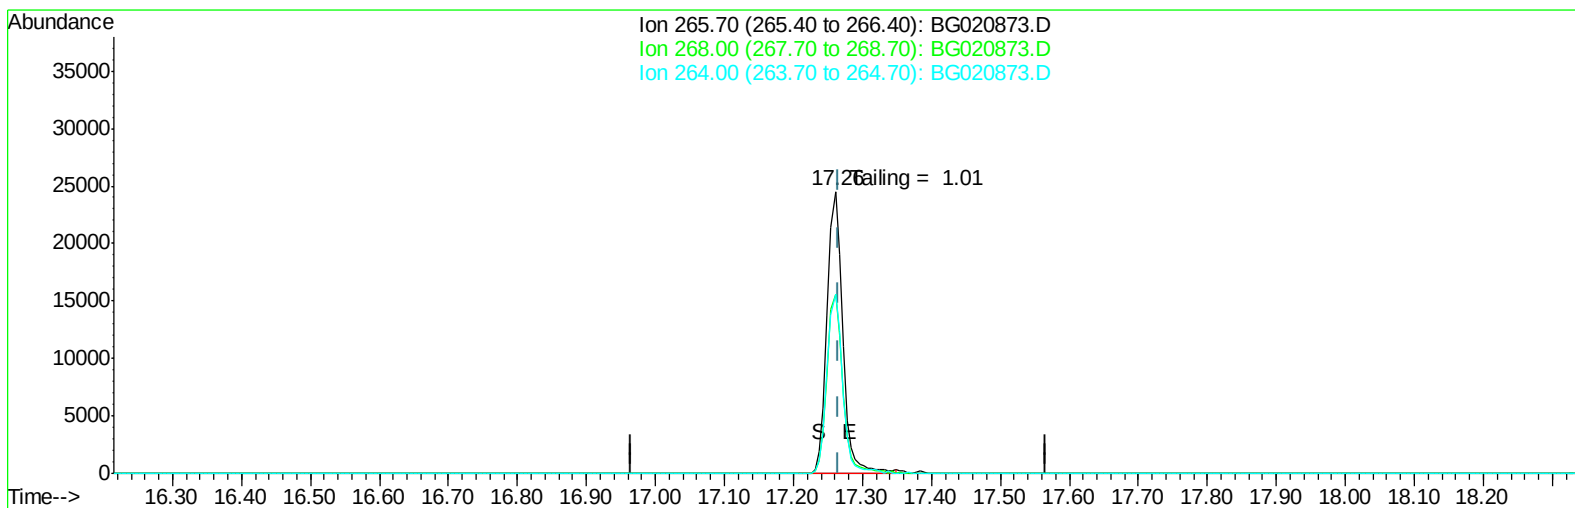

TIC: BG020873.D

(69) Pentachlorophenol (C)




17.261min (-0.005) 14746.85ng

response 38480

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	63.45
264.00	62.80	63.48
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG021116\
Data File : BG020873.D
Acq On : 12 Feb 2016 1:59
Operator : SJ/UM
Sample : DFTPP
Misc : L00 20PPM
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:31:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

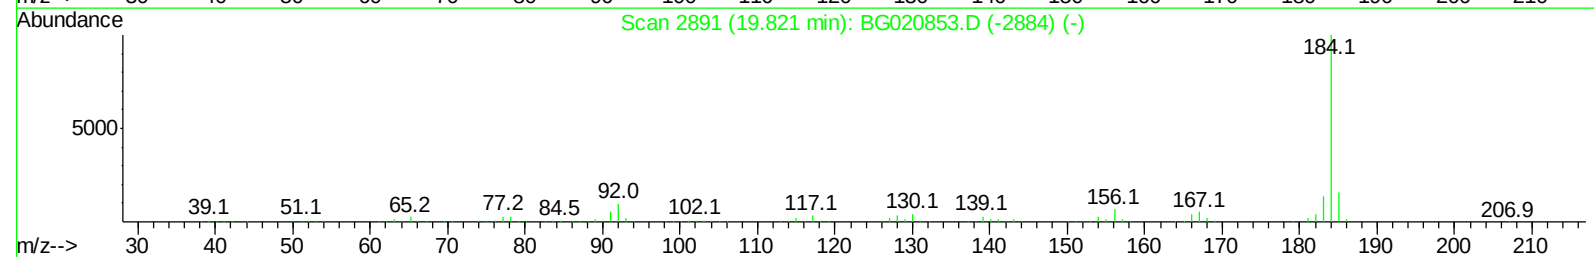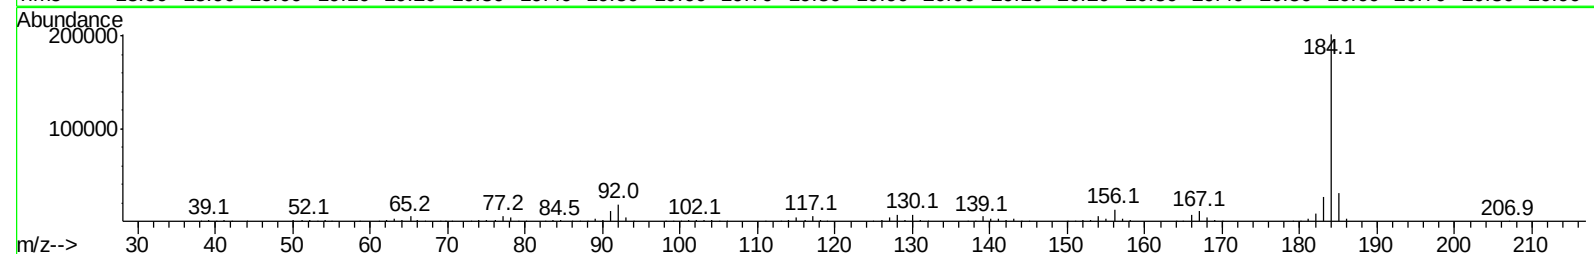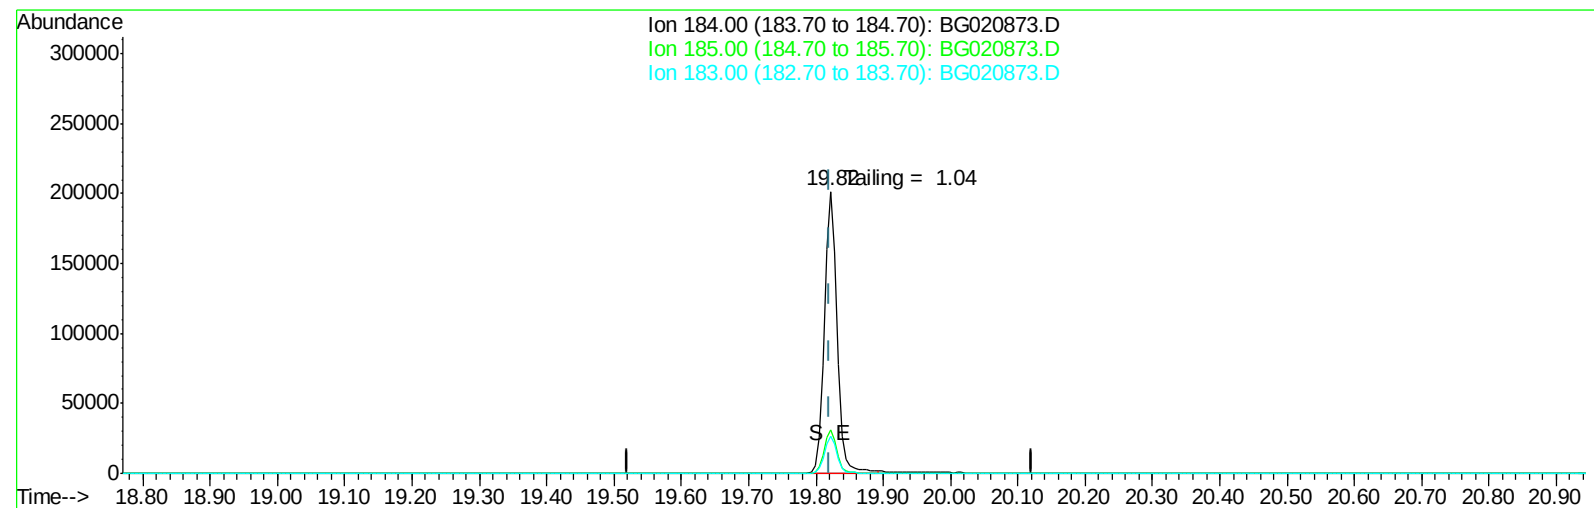

TIC: BG020873.D

(76) Benzidine

19.822min (+0.001) 0.00ng

response 273804

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.48
183.00	13.70	13.34
0.00	0.00	0.00