


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG021116\
 Data File : BG020859.D
 Acq On : 11 Feb 2016 16:51
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 15:26:53 2016

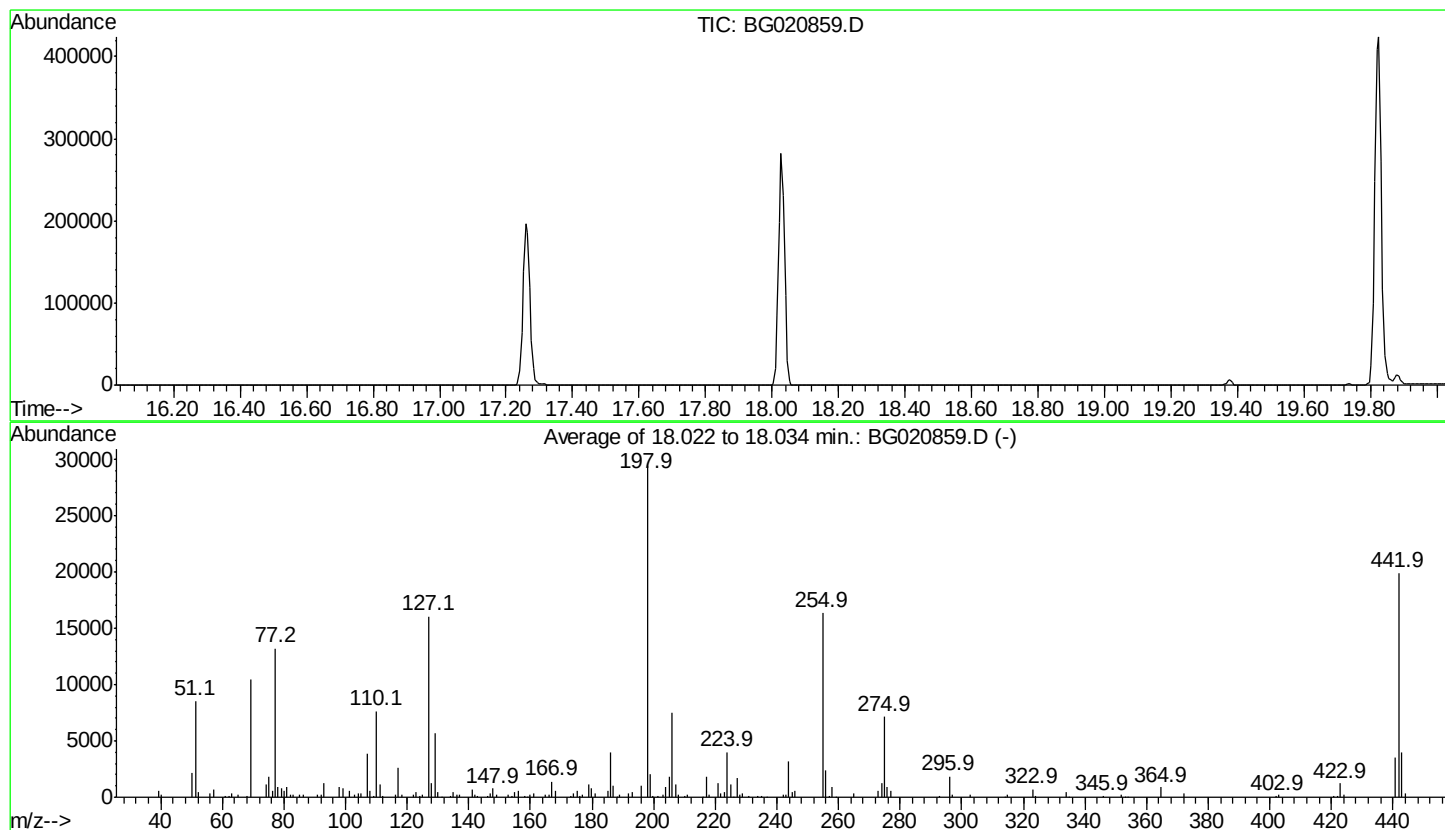

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	8577	PASS
68	69	0.00	2	0.8	82	PASS
69	198	0.00	100	35.6	10459	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	16023	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29418	PASS
199	198	5	9	7.1	2100	PASS
275	198	10	60	24.2	7108	PASS
365	198	1	100	3.0	891	PASS
441	442	0.01	24	17.6	3499	PASS
442	198	50	100	67.7	19905	PASS
443	442	15	24	19.8	3948	PASS