


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG021116\
 Data File : BG020873.D
 Acq On : 12 Feb 2016 1:59
 Operator : SJ/UM
 Sample : DFTPP
 Misc : L00 20PPM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 15:26:53 2016

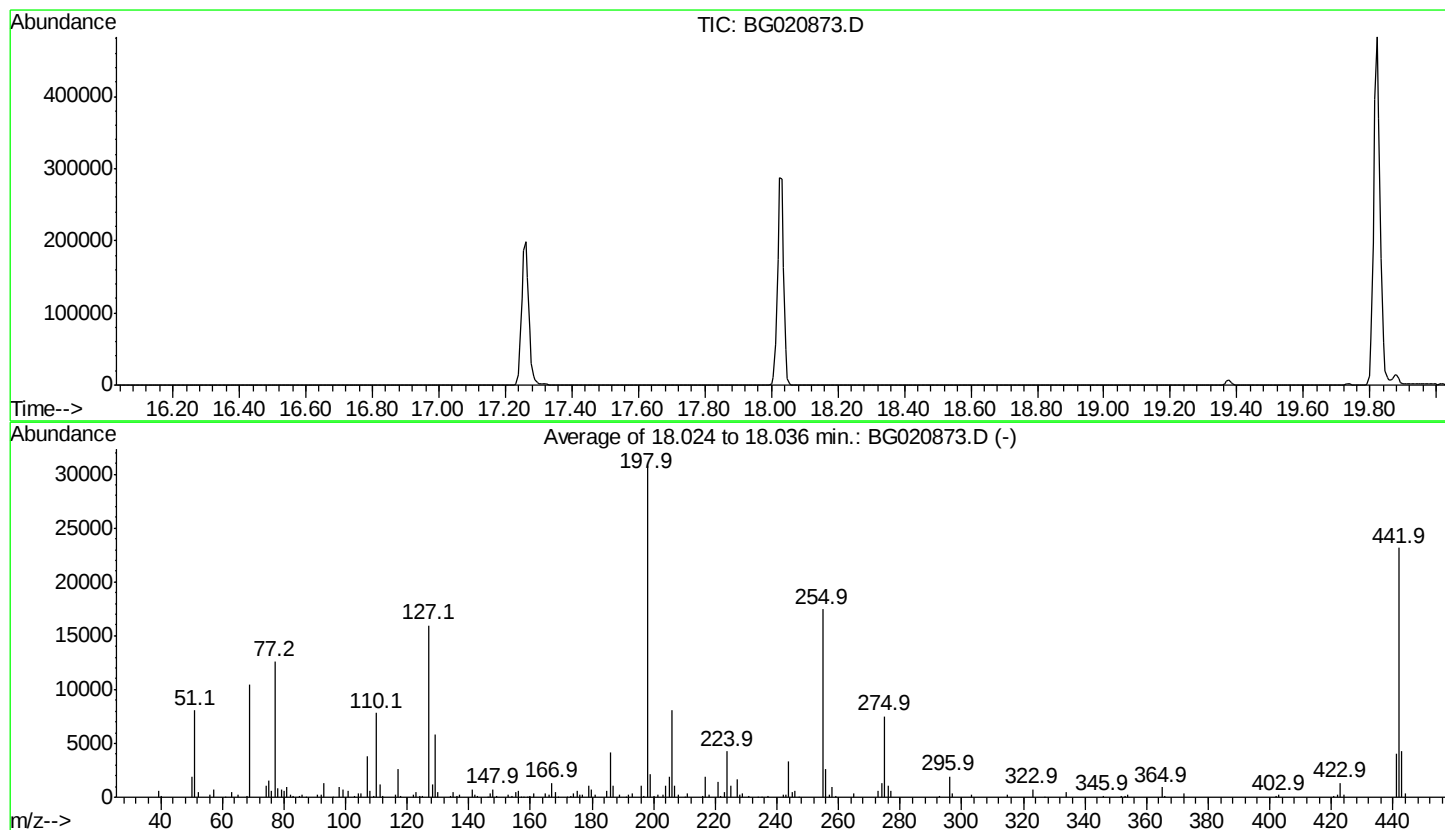

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	8045	PASS
68	69	0.00	2	0.6	67	PASS
69	198	0.00	100	34.0	10464	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	15989	PASS
197	198	0.00	2	0.2	68	PASS
198	198	100	100	100.0	30794	PASS
199	198	5	9	7.0	2156	PASS
275	198	10	60	24.3	7496	PASS
365	198	1	100	3.0	913	PASS
441	442	0.01	24	17.6	4077	PASS
442	198	50	100	75.1	23141	PASS
443	442	15	24	18.6	4315	PASS