
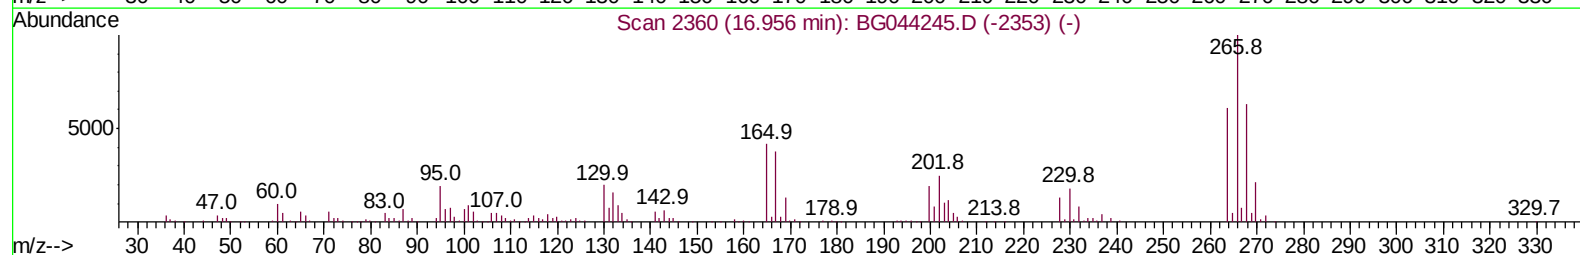
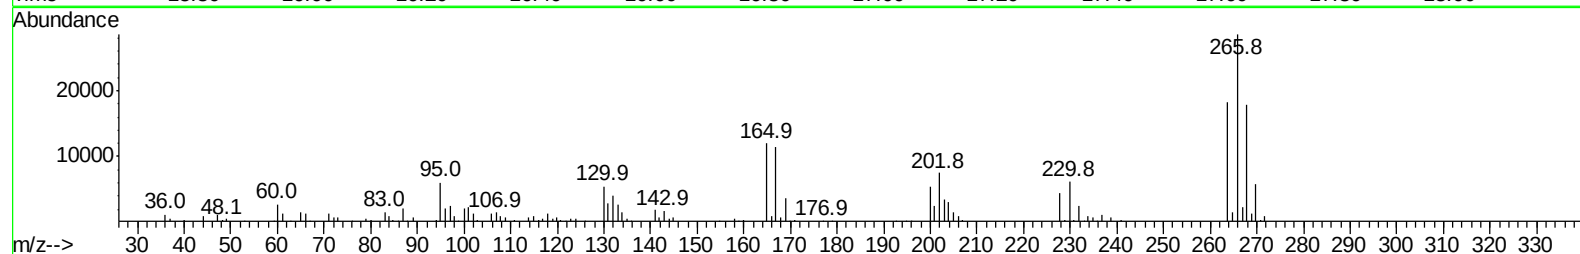


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021120\
 Data File : BG044385.D
 Acq On : 11 Feb 2020 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 10:49:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

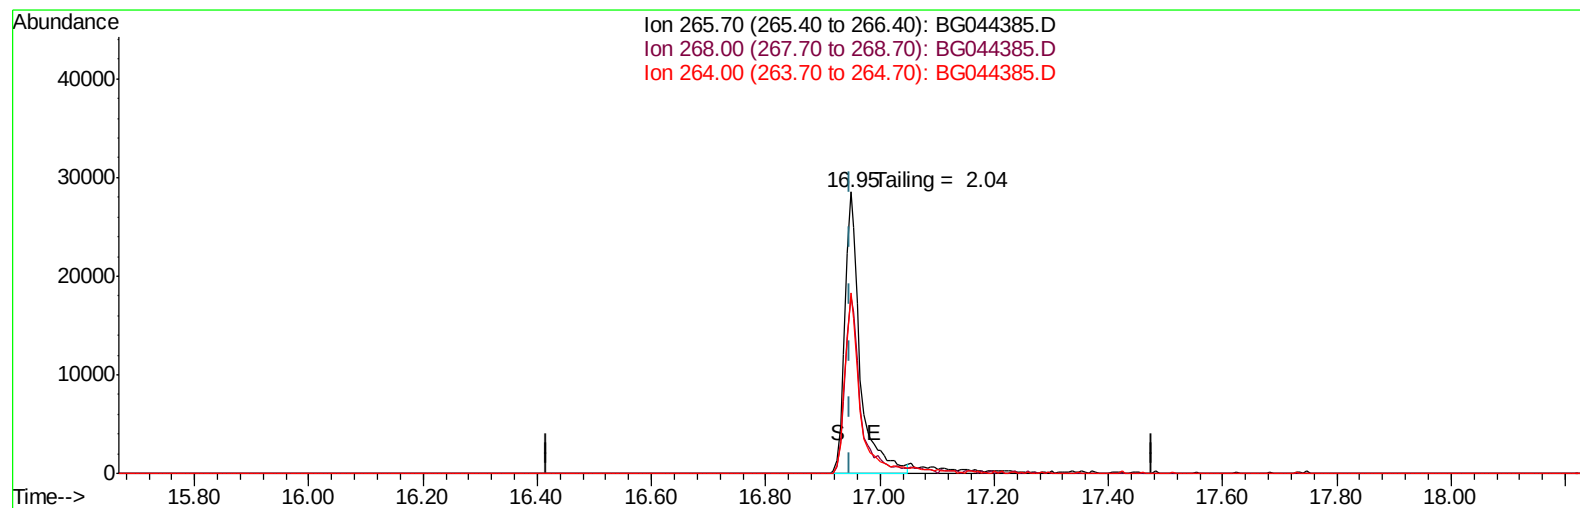

TIC: BG044385.D

(70) Pentachlorophenol (C)




16.948min (+0.000) 19872.79ng

response 53105

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.68
264.00	60.90	64.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021120\
 Data File : BG044385.D
 Acq On : 11 Feb 2020 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 10:49:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

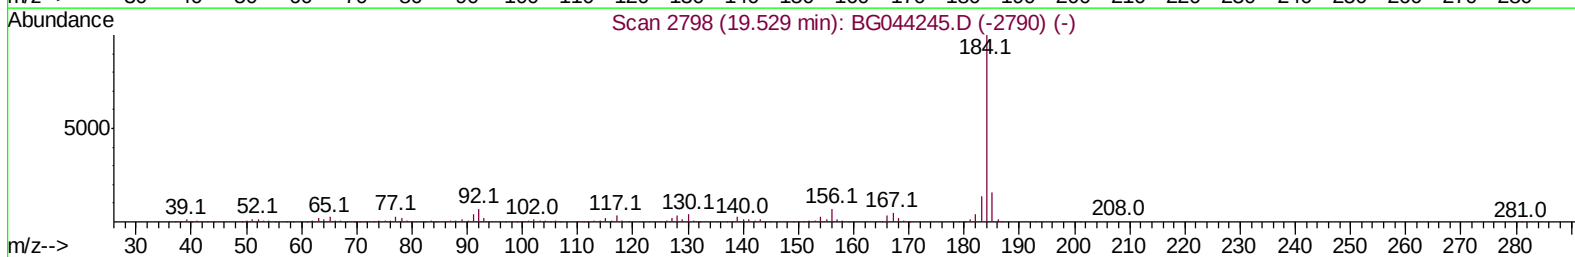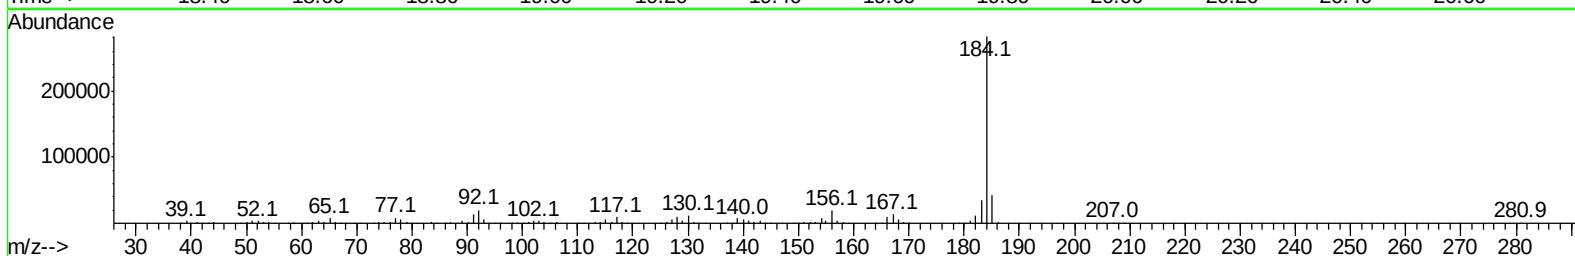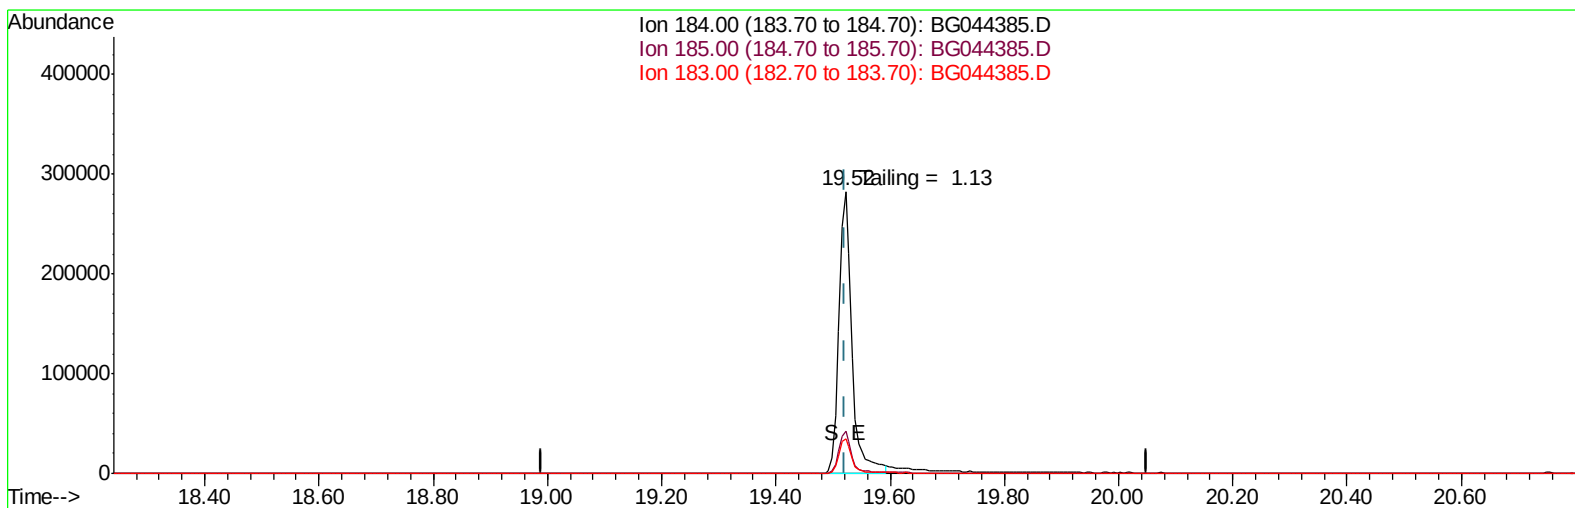

TIC: BG044385.D

(77) Benzidine

19.522min (+0.000) 0.00ng

response 479135

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.81
183.00	13.50	12.42
0.00	0.00	0.00