


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021120\
 Data File : BG044385.D
 Acq On : 11 Feb 2020 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

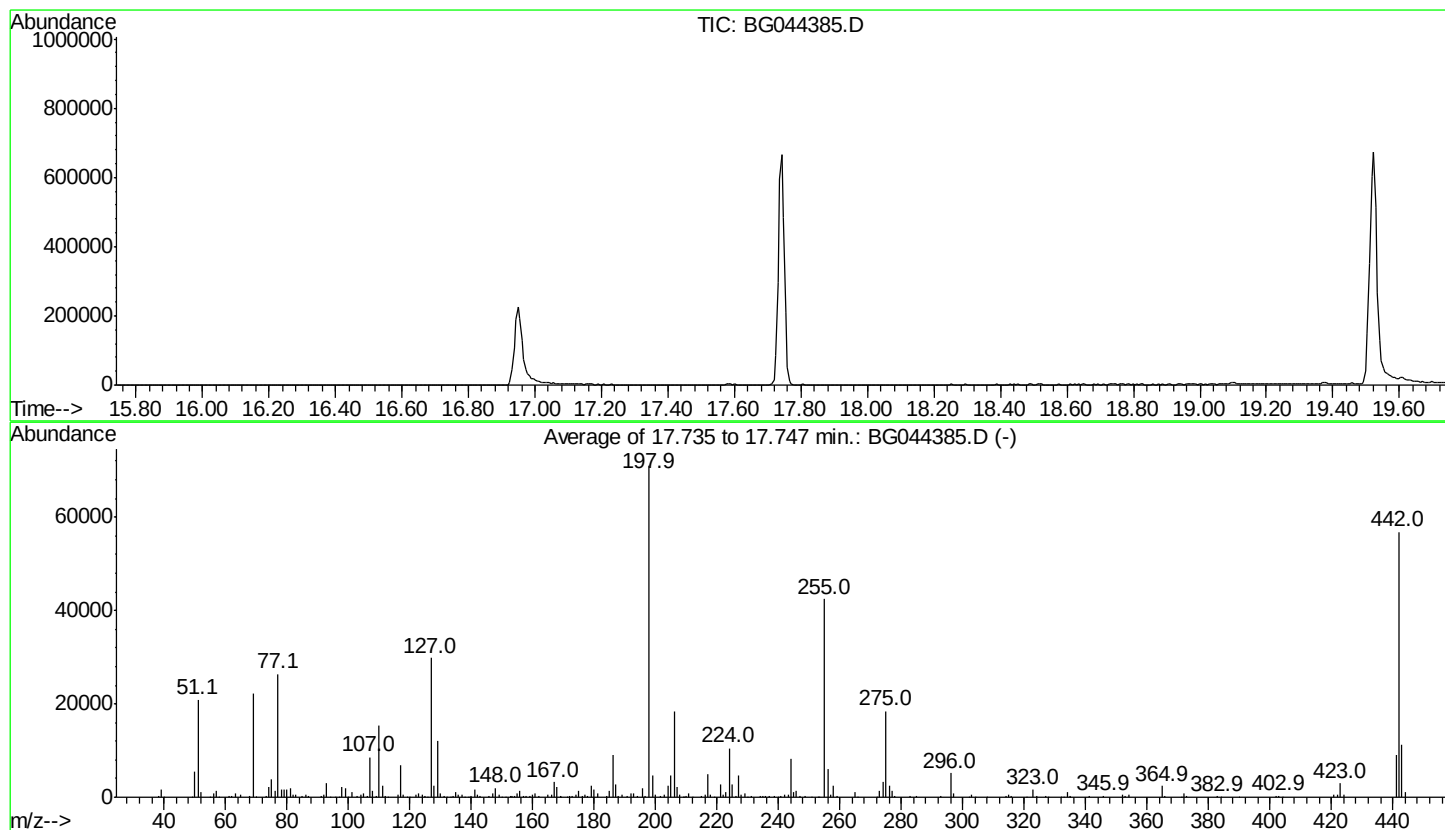

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	20869	PASS
68	69	0.00	2	0.9	196	PASS
69	198	0.00	100	31.1	22124	PASS
70	69	0.00	2	0.2	54	PASS
127	198	10	80	42.0	29840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71042	PASS
199	198	5	9	6.5	4635	PASS
275	198	10	60	25.9	18392	PASS
365	198	1	100	3.3	2354	PASS
441	198	0.01	100	12.6	8955	PASS
442	198	50	100	80.1	56882	PASS
443	442	15	24	19.8	11249	PASS