
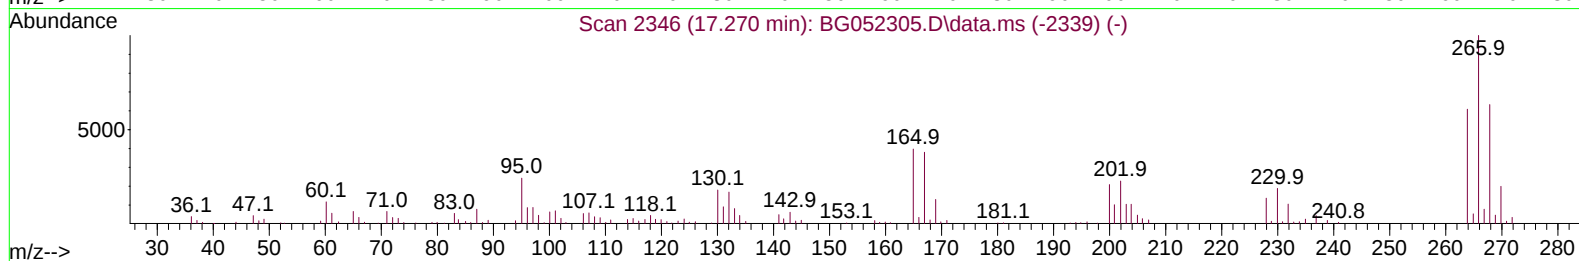
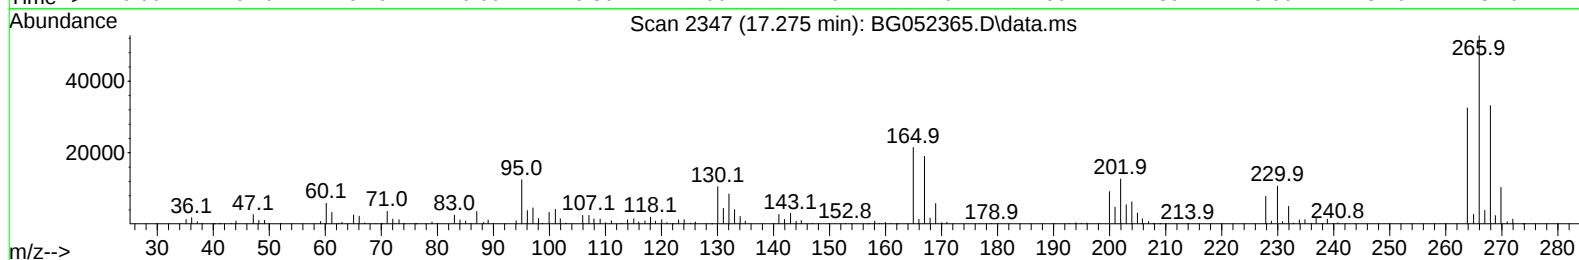


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021122\
Data File : BG052365.D
Acq On : 11 Feb 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 11:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

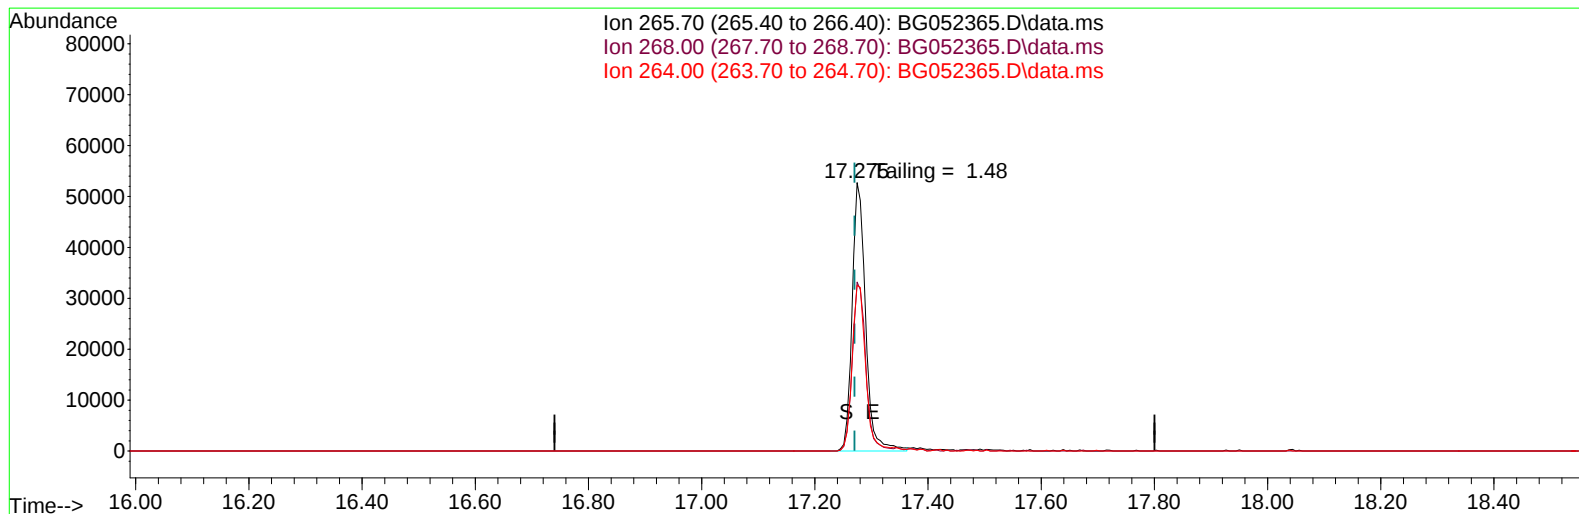

TIC: BG052365.D\data.ms

(70) Pentachlorophenol (C)




17.275min (+ 0.005) 235943.02 ng

response 88305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.95
264.00	65.20	61.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021122\
Data File : BG052365.D
Acq On : 11 Feb 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 11:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

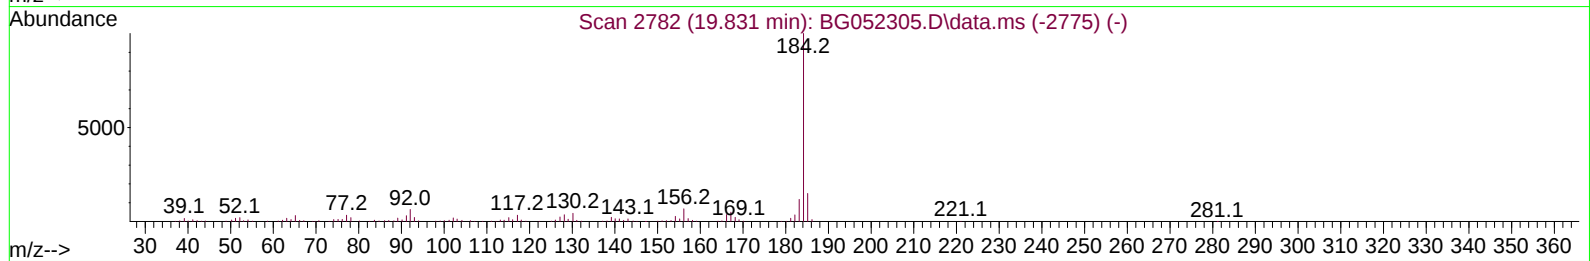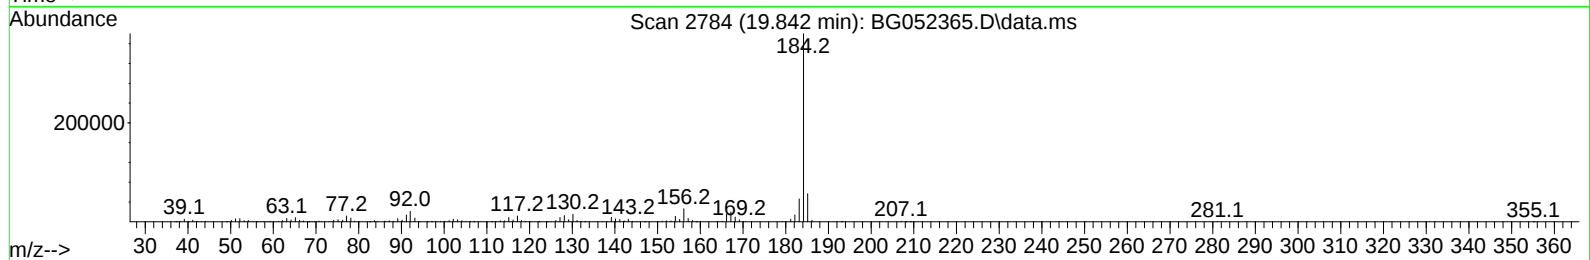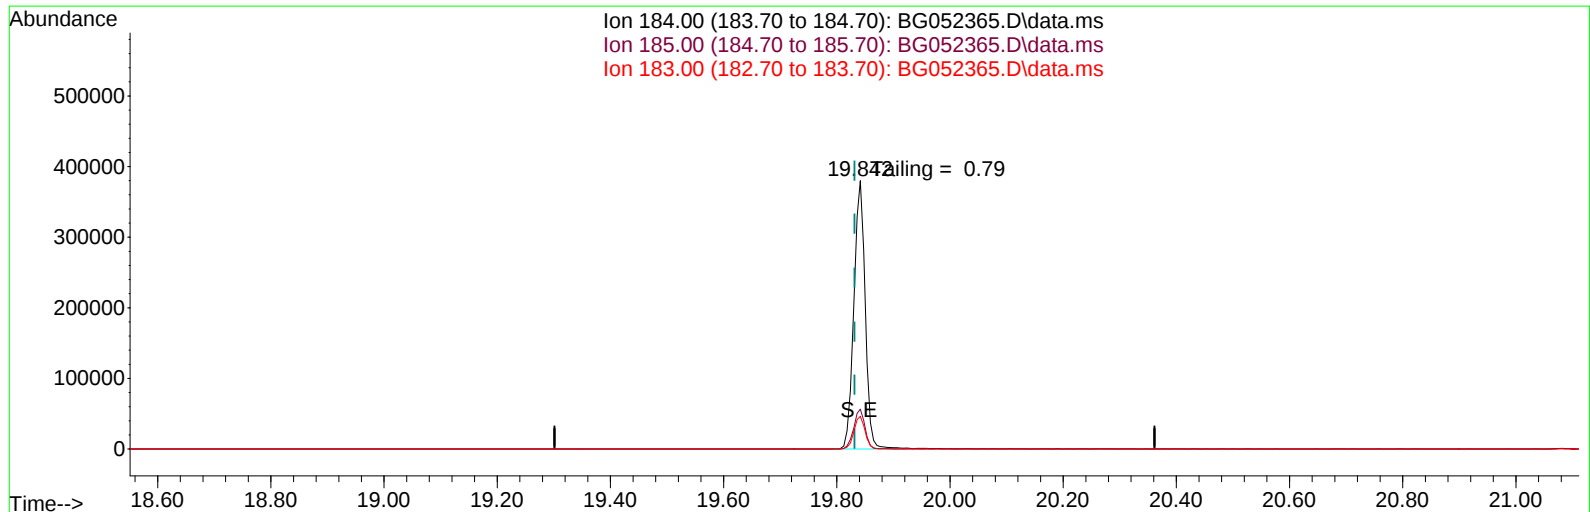

TIC: BG052365.D\data.ms

(77) Benzidine

19.842min (+ 0.010) 212182.50 ng

response 530462

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.89
183.00	12.20	12.21
0.00	0.00	0.00