
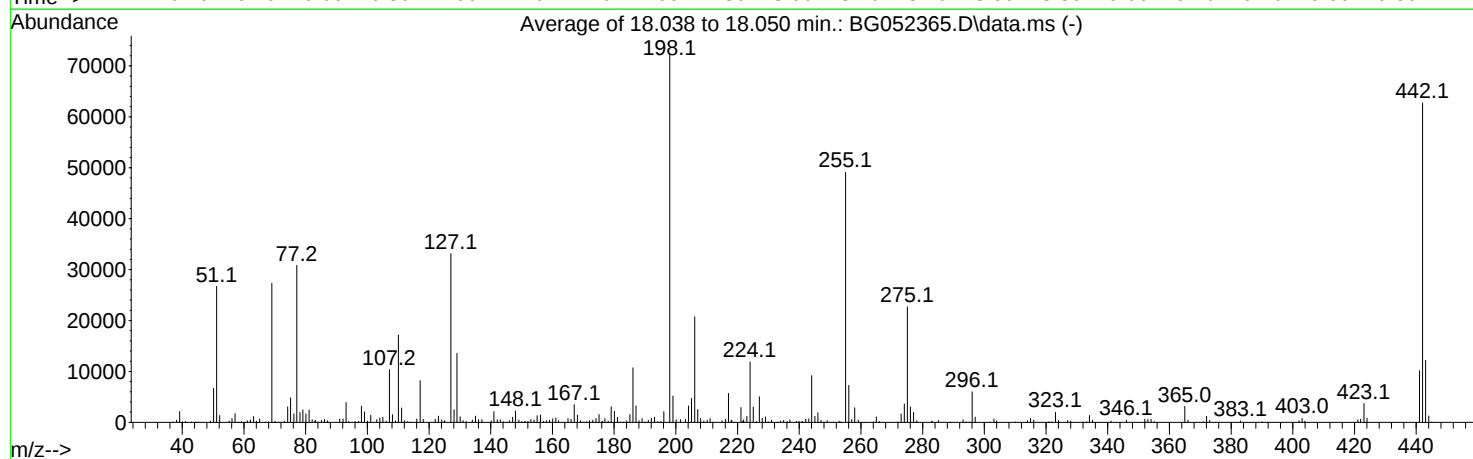


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021122\
 Data File : BG052365.D
 Acq On : 11 Feb 2022 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

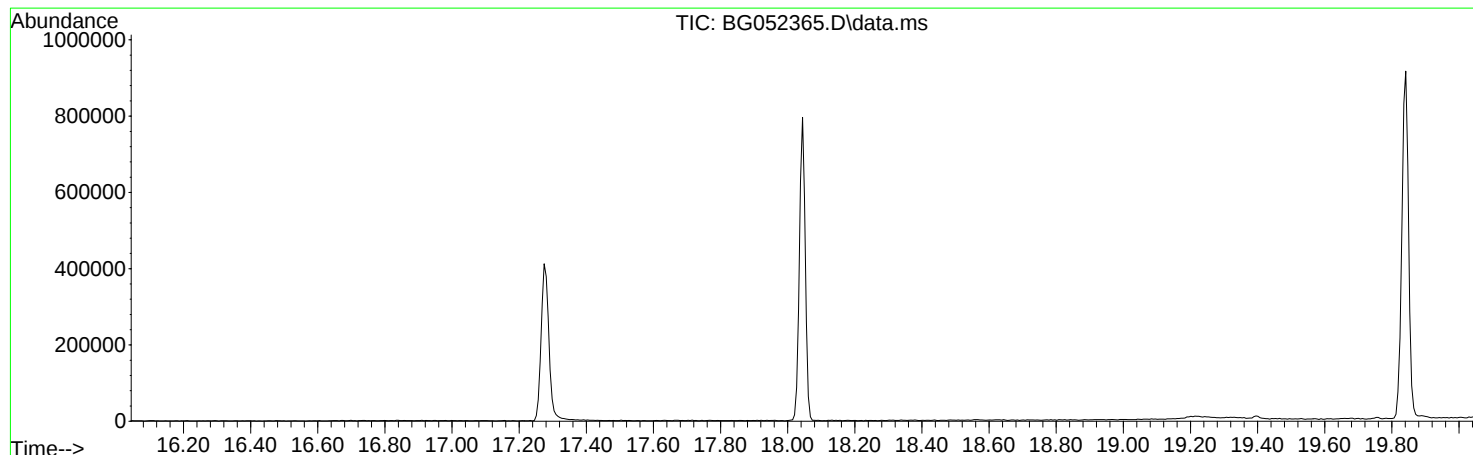

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	26696	PASS
68	69	0.00	2	0.5	129	PASS
69	198	0.00	100	37.8	27315	PASS
70	69	0.00	2	0.9	233	PASS
127	198	10	80	45.9	33147	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72240	PASS
199	198	5	9	7.2	5177	PASS
275	198	10	60	31.4	22677	PASS
365	198	1	100	4.3	3128	PASS
441	198	0.01	100	14.0	10141	PASS
442	442	50	100	100.0	62704	PASS
443	442	15	24	19.4	12171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/11/2022	BNA_G	<u>BG052365.D</u>
Compound Name	Response	Retention Time
DDT	283871	21.08
DDD	2942	20.62
DDE	388	20.12
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3330	287201	1.16

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021122\
Data File : BG052365.D
Acq On : 11 Feb 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 11 11:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

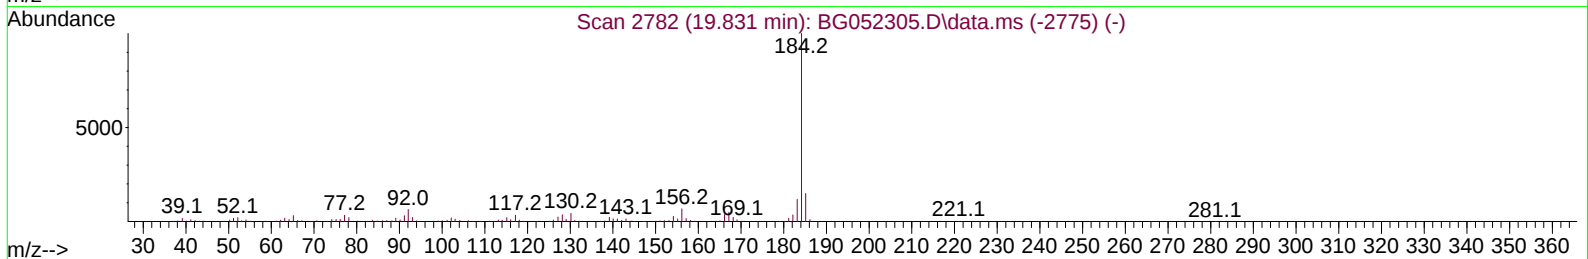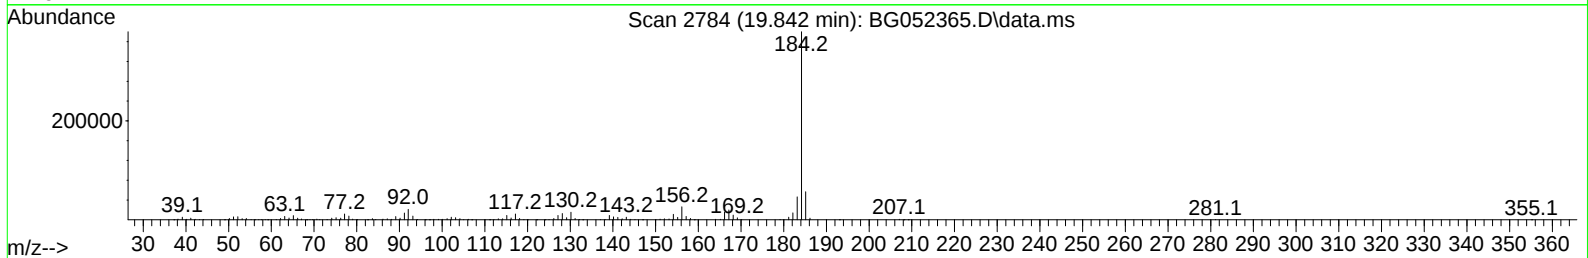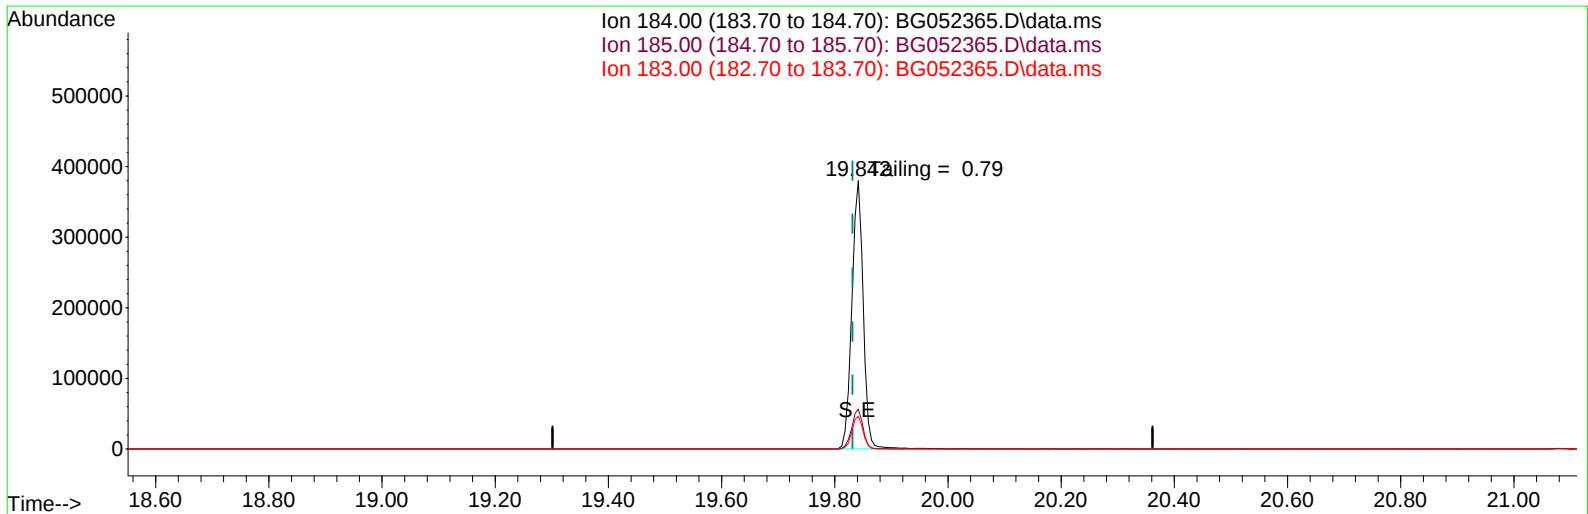

TIC: BG052365.D\data.ms

(77) Benzidine

19.842min (+ 0.010) 212182.50 ng

response 530462

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.89
183.00	12.20	12.21
0.00	0.00	0.00