


Data Path : U:\HPCHEM1\BNA G\DATA\BG021216\  
 Data File : BG020890.D  
 Acq On : 12 Feb 2016 13:16  
 Operator : SJ/UM  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\625-TERPINEOL-BG021216.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Feb 12 18:22:09 2016

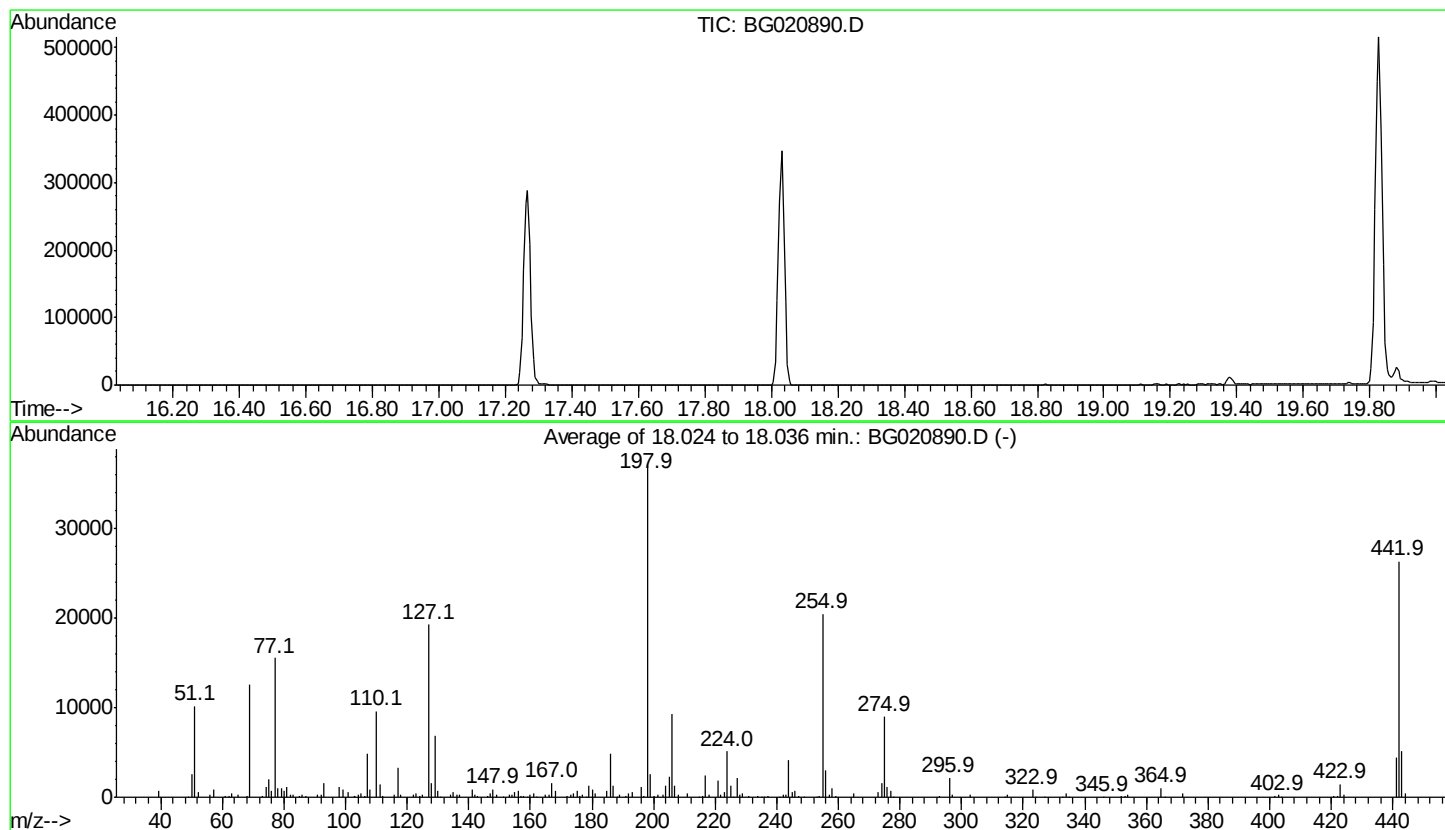

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2579

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 30           | 60           | 27.5      | 10193   | FAIL*            |
| 68          | 69           | 0.00         | 2            | 0.9       | 107     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.9      | 12551   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 40           | 60           | 52.0      | 19248   | PASS             |
| 197         | 198          | 0.00         | 1            | 0.5       | 195     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 37034   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 2519    | PASS             |
| 275         | 198          | 10           | 30           | 24.2      | 8975    | PASS             |
| 365         | 198          | 1            | 100          | 2.8       | 1048    | PASS             |
| 441         | 443          | 0.01         | 100          | 86.1      | 4405    | PASS             |
| 442         | 198          | 40           | 100          | 71.1      | 26349   | PASS             |
| 443         | 442          | 17           | 23           | 19.4      | 5116    | PASS             |