



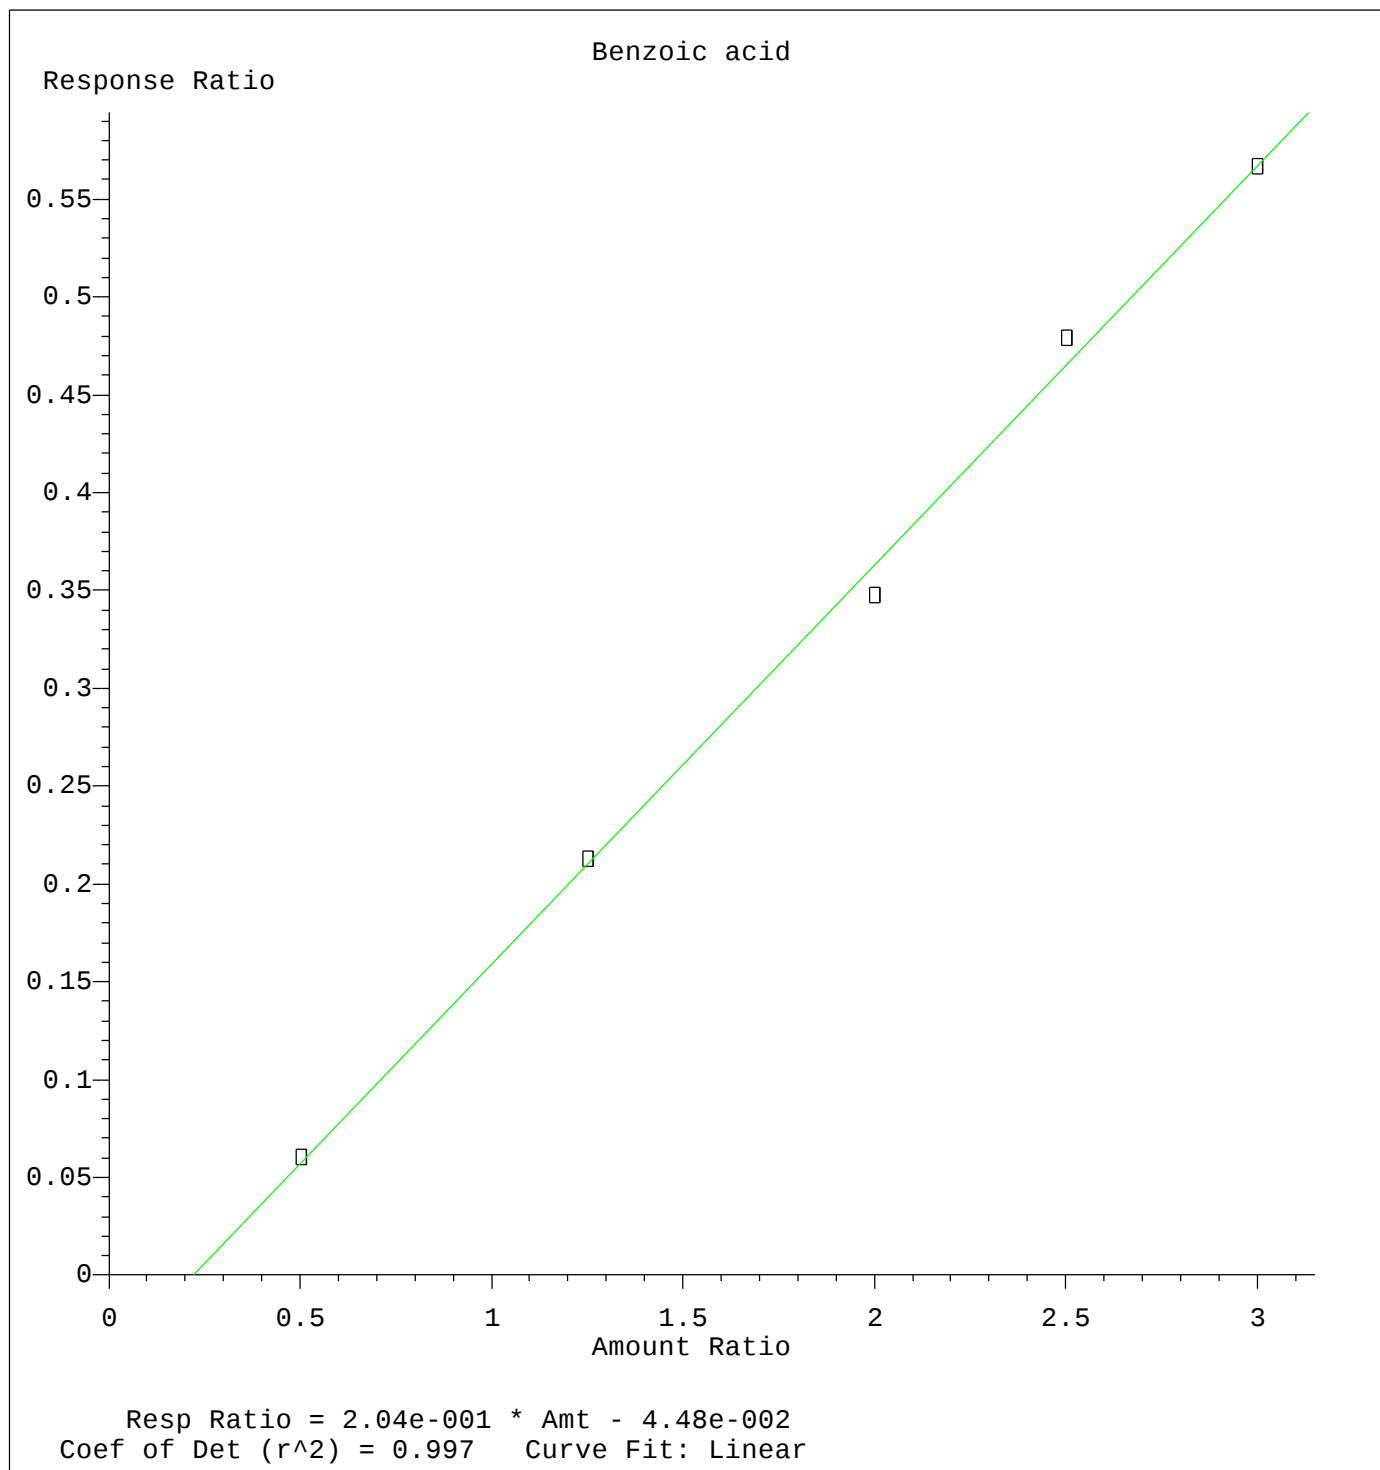

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021218.M  
Calibration Table Last Updated: Fri Feb 16 18:34:49 2018


# 2,4-Dinitrophenol

Response Ratio

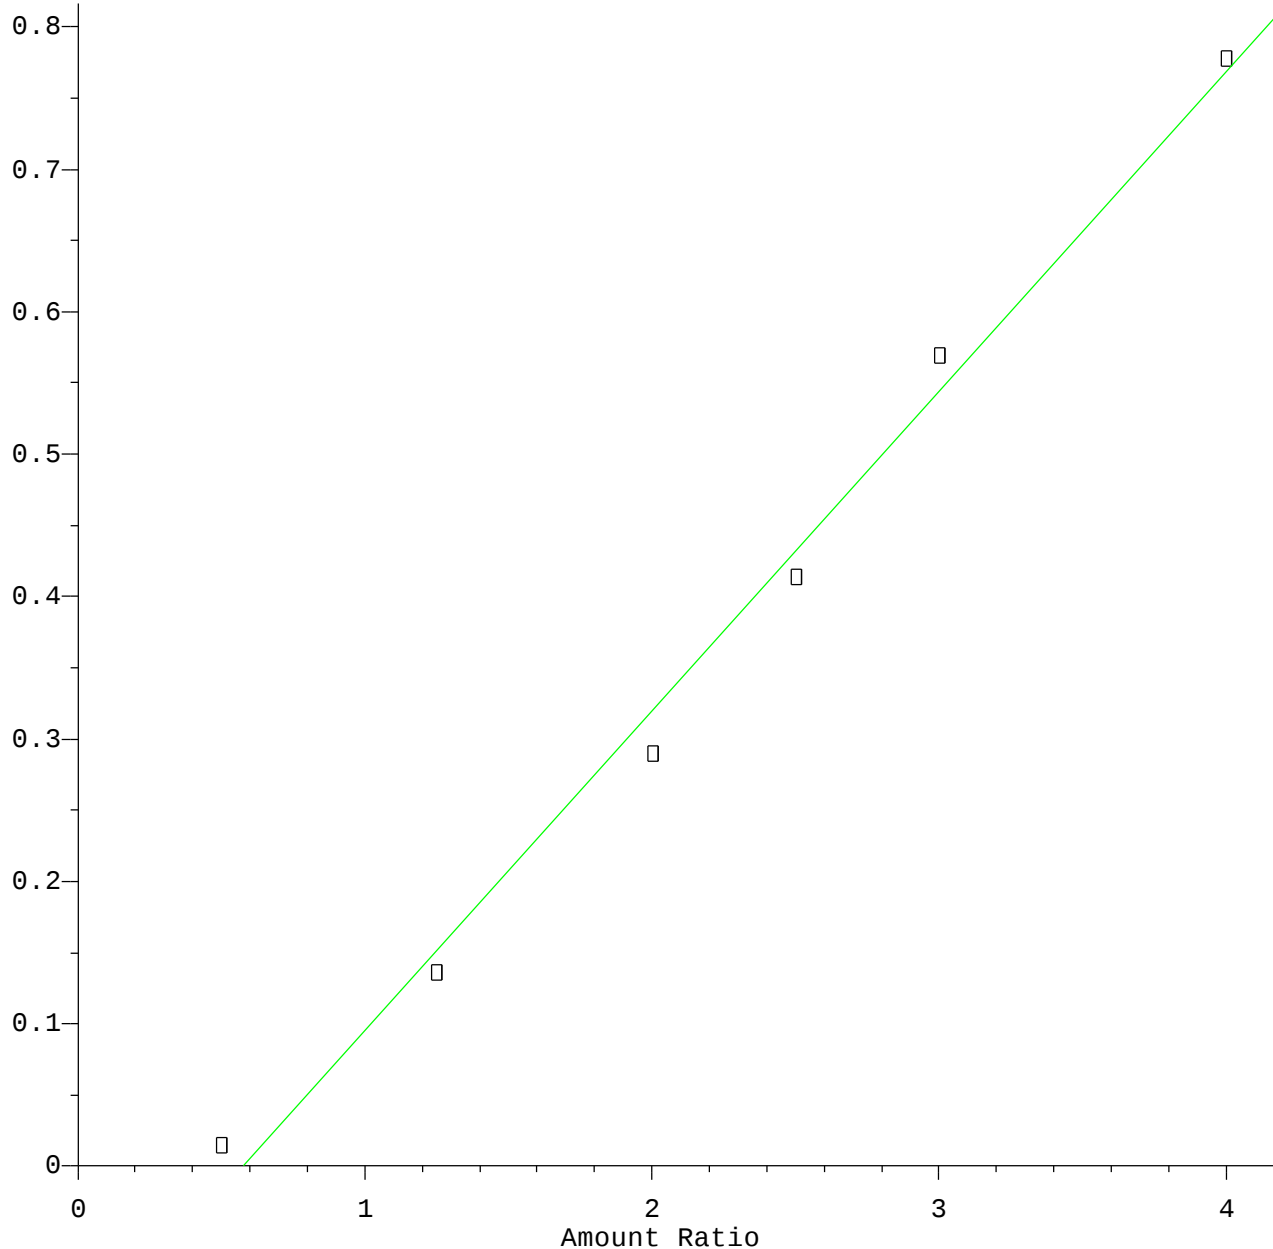


Resp Ratio =  $2.24 \times 10^{-1} \times \text{Amt} - 1.28 \times 10^{-1}$   
Coef of Det ( $r^2$ ) = 0.992    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021218.M  
Calibration Table Last Updated: Fri Feb 16 18:34:49 2018

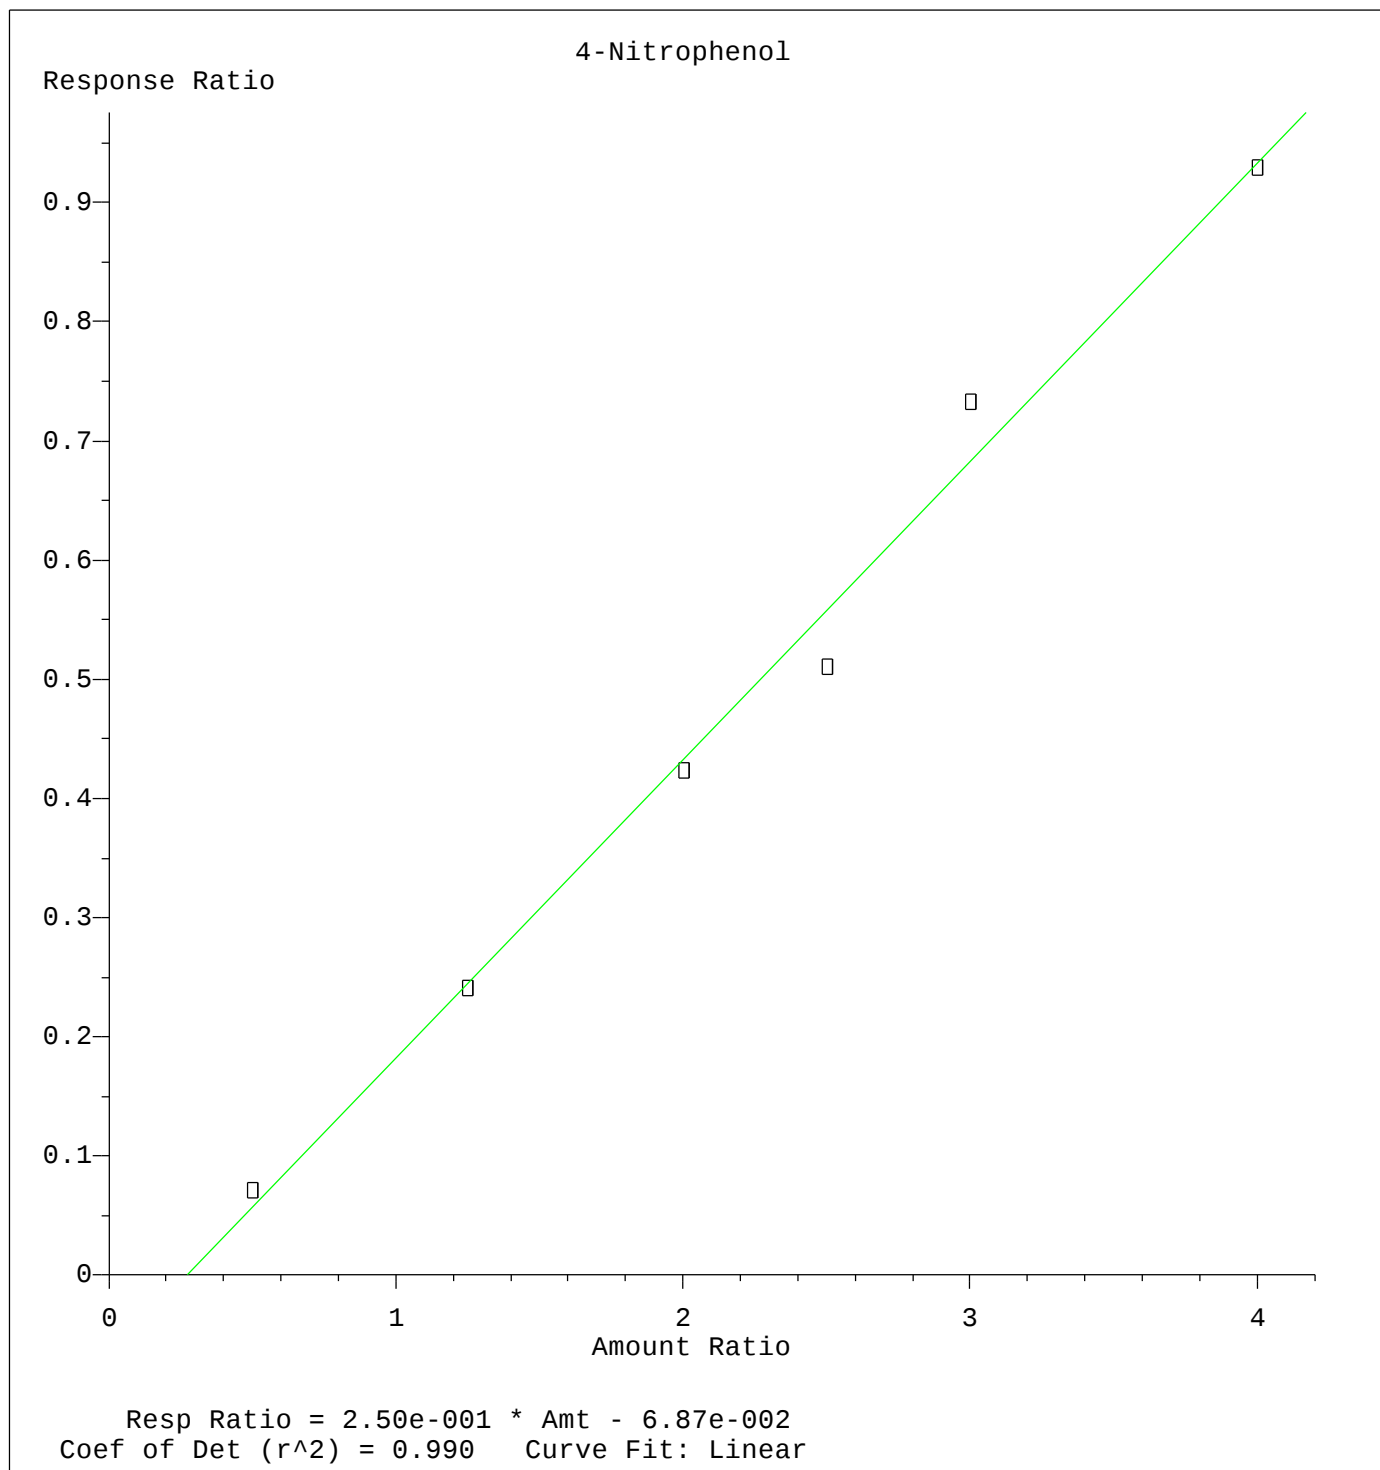

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021218.M  
Calibration Table Last Updated: Fri Feb 16 18:34:49 2018

4,6-Dinitro-2-methylphenol

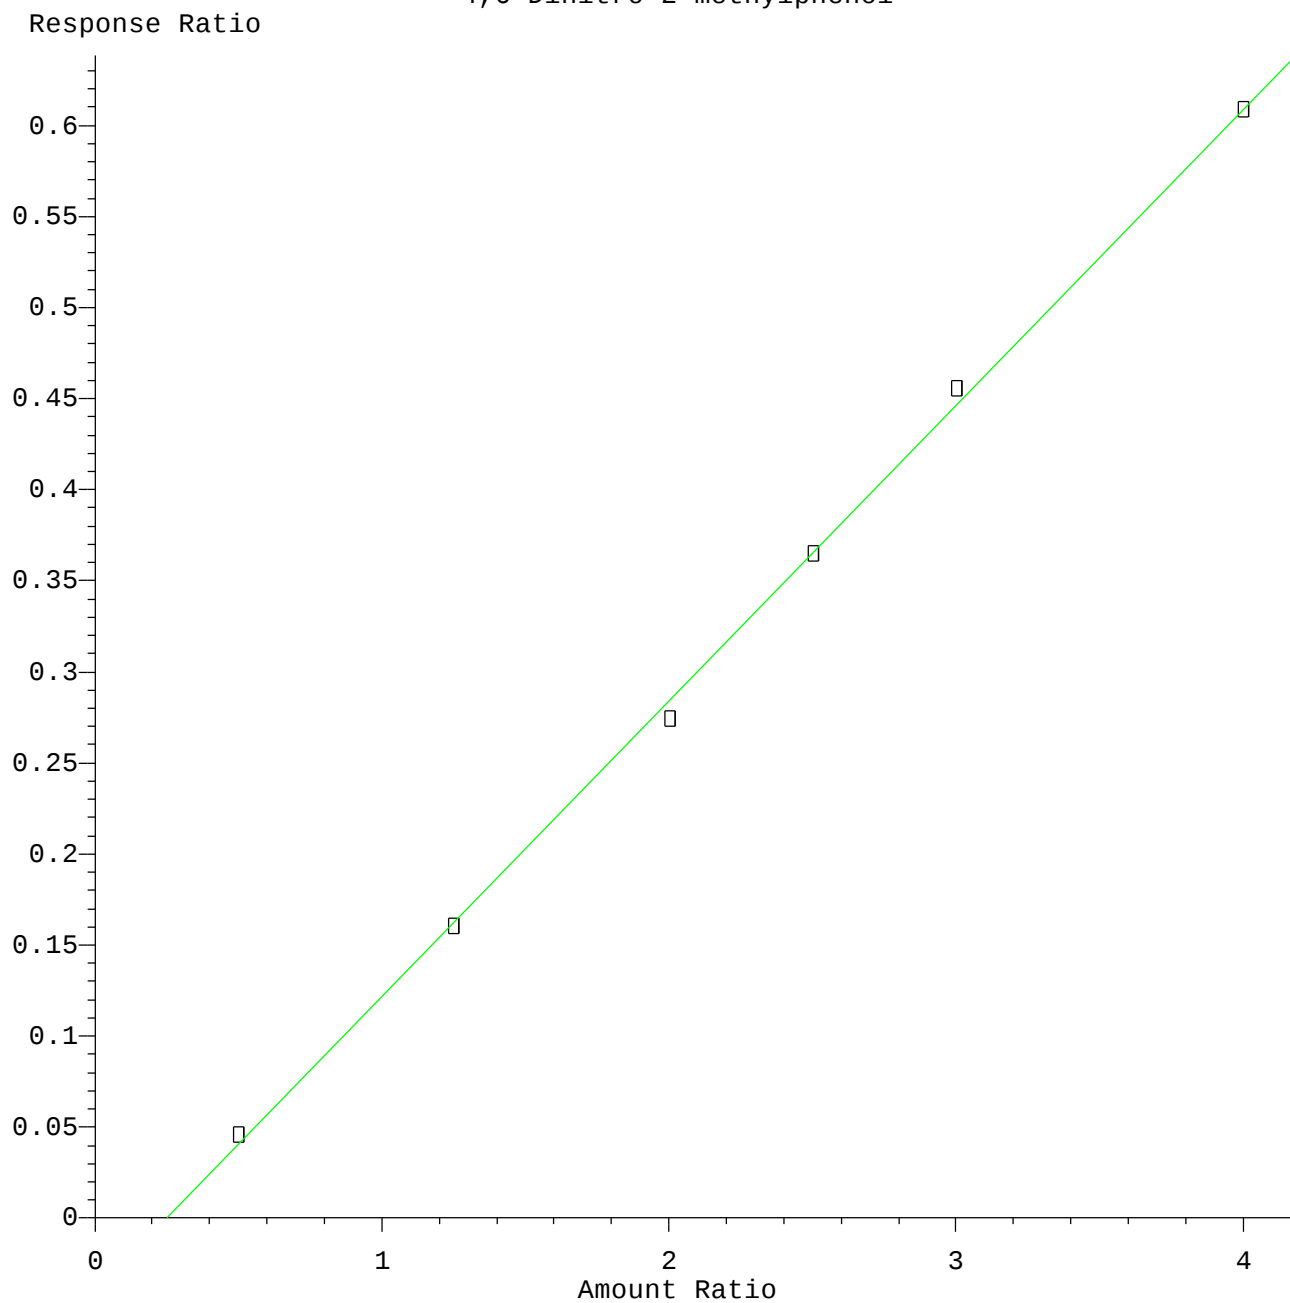

Resp Ratio =  $1.62 \times 10^{-1} \times \text{Amt} - 4.08 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021218.M  
Calibration Table Last Updated: Fri Feb 16 18:34:49 2018