


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021218\
 Data File : BG032645.D
 Acq On : 12 Feb 2018 12:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 18:34:49 2018

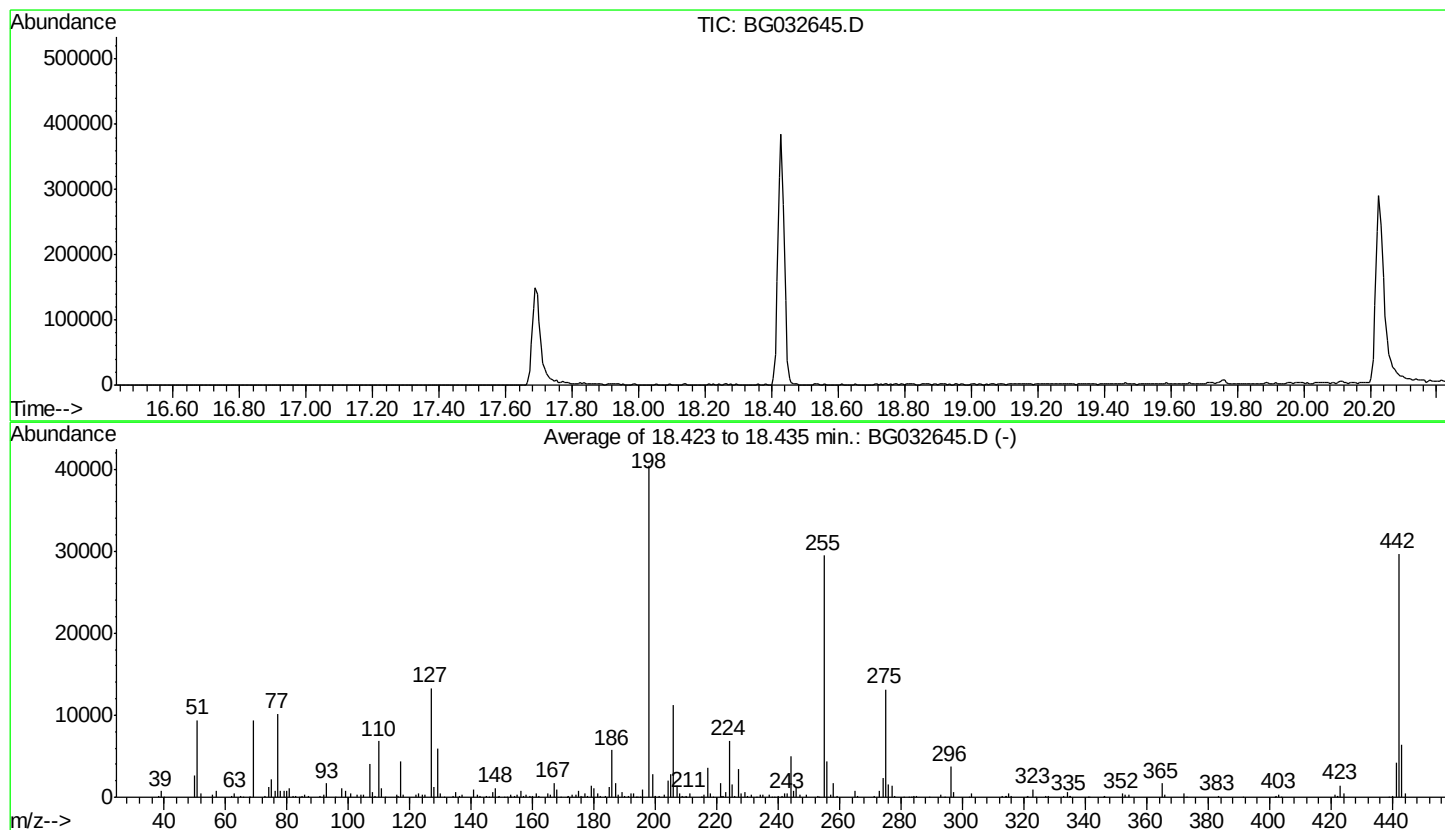

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	9404	PASS
68	69	0.00	2	0.9	80	PASS
69	198	0.00	100	23.1	9344	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.9	13308	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40413	PASS
199	198	5	9	7.1	2868	PASS
275	198	10	60	32.4	13113	PASS
365	198	1	100	4.1	1656	PASS
441	442	0.01	24	14.4	4282	PASS
442	198	50	100	73.4	29648	PASS
443	442	15	24	21.4	6338	PASS