
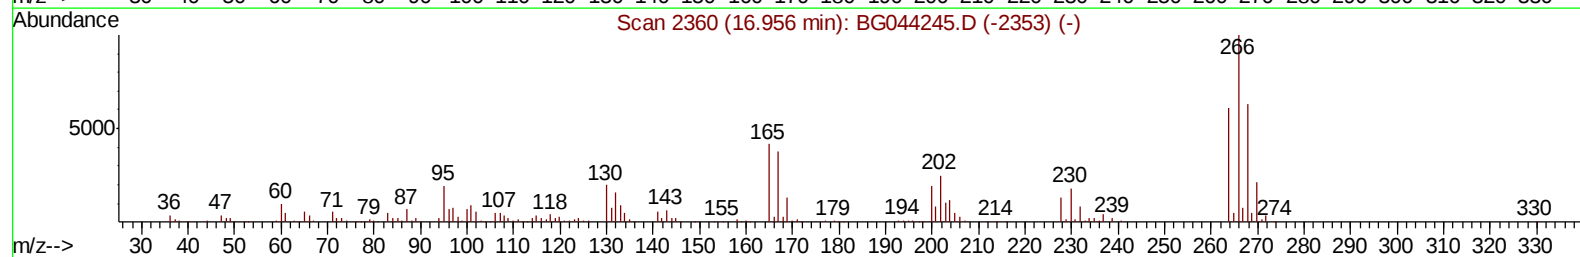
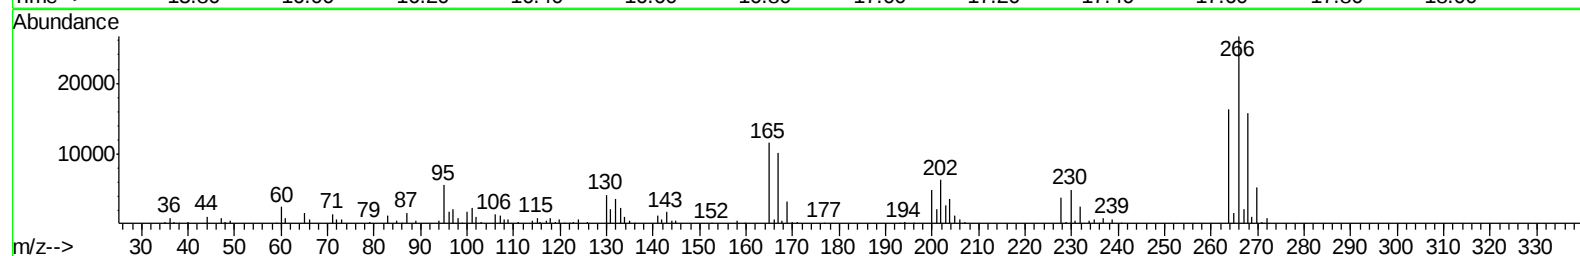


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021220\
 Data File : BG044404.D
 Acq On : 12 Feb 2020 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 03:13:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

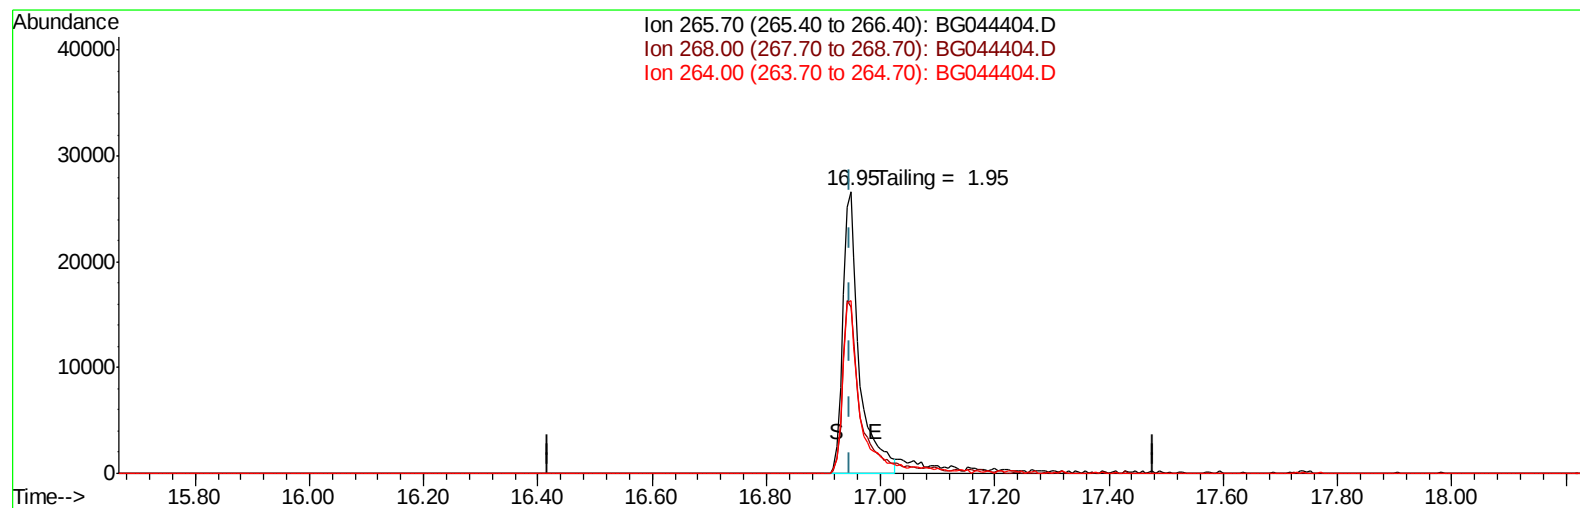

TIC: BG044404.D

(70) Pentachlorophenol (C)




16.947min (-0.001) 23630.58ng

response 55103

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	58.90
264.00	60.90	61.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021220\
 Data File : BG044404.D
 Acq On : 12 Feb 2020 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 03:13:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

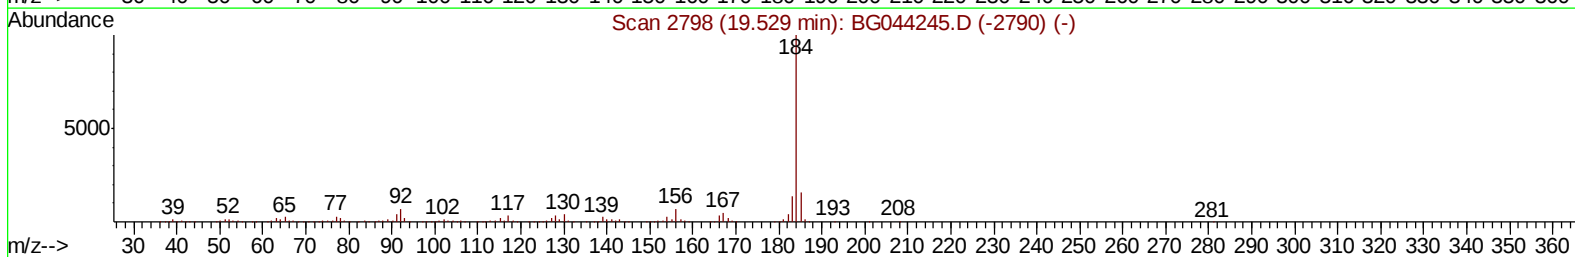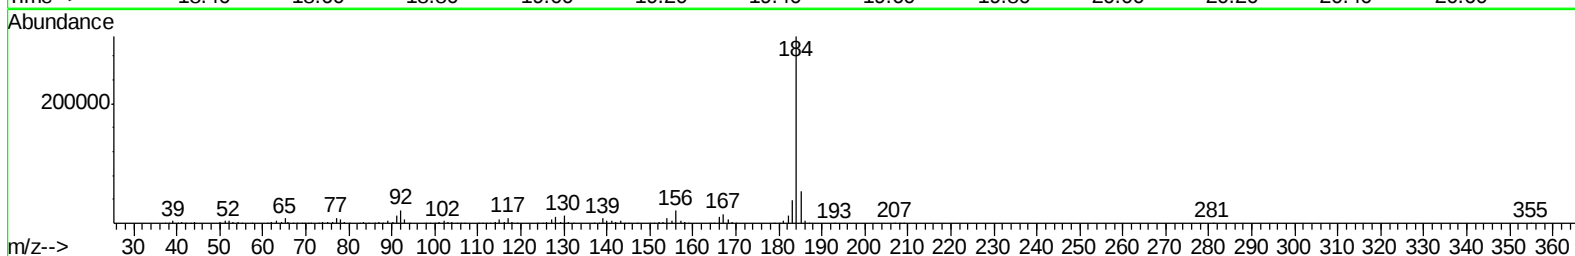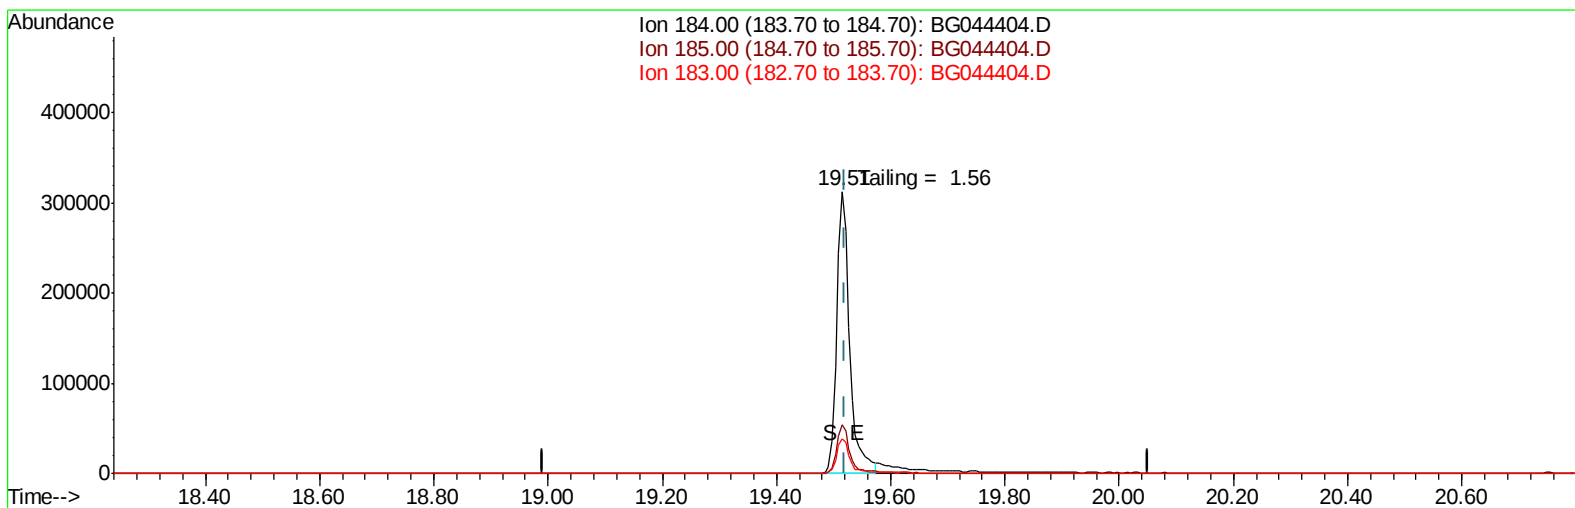

TIC: BG044404.D

(77) Benzidine

19.515min (-0.006) 0.00ng

response 527082

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	17.11
183.00	13.50	12.51
0.00	0.00	0.00