

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021220\
 Data File : BG044410.D
 Acq On : 12 Feb 2020 15:51
 Operator : CG/JU
 Sample : L1491-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-1E-(7.5-9.5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.479	400	407	419	rBV	912203	1500183	39.38%	7.449%
2	7.072	670	678	692	rBV	946516	1663969	43.68%	8.262%
3	7.900	812	819	828	rBV	225952	376682	9.89%	1.870%
4	8.223	865	874	883	rBV	747194	1300840	34.15%	6.459%
5	9.058	1008	1016	1030	rBV	556655	1035052	27.17%	5.139%
6	10.703	1287	1296	1308	rBV	298145	557127	14.63%	2.766%
7	13.165	1707	1715	1727	rBV	1535905	2544121	66.79%	12.632%
8	13.993	1849	1856	1866	rBV	39112	70608	1.85%	0.351%
9	14.539	1941	1949	1957	rBV	557152	877653	23.04%	4.358%
10	16.026	2196	2202	2220	rBV	1347820	2154167	56.55%	10.696%
11	17.283	2409	2416	2429	rBV	748228	1144095	30.04%	5.681%
12	19.898	2855	2861	2875	rBV	2803194	3809163	100.00%	18.913%
13	21.202	3078	3083	3091	rBV2	48406	90016	2.36%	0.447%
14	21.525	3131	3138	3150	rBV	753232	1257583	33.01%	6.244%
15	22.319	3266	3273	3283	rVB2	36404	81777	2.15%	0.406%
16	22.648	3324	3329	3338	rBV6	14557	41075	1.08%	0.204%
17	22.988	3382	3387	3395	rVB2	45452	86094	2.26%	0.427%
18	23.752	3512	3517	3529	rVB2	52727	101107	2.65%	0.502%
19	24.610	3652	3663	3683	rBV2	445681	1358474	35.66%	6.745%
20	25.738	3846	3855	3866	rBV3	27646	90293	2.37%	0.448%


Sum of corrected areas: 20140079

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021220\
Data File : BG044410.D
Acq On : 12 Feb 2020 15:51
Operator : CG/JU
Sample : L1491-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1E-(7.5-9.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

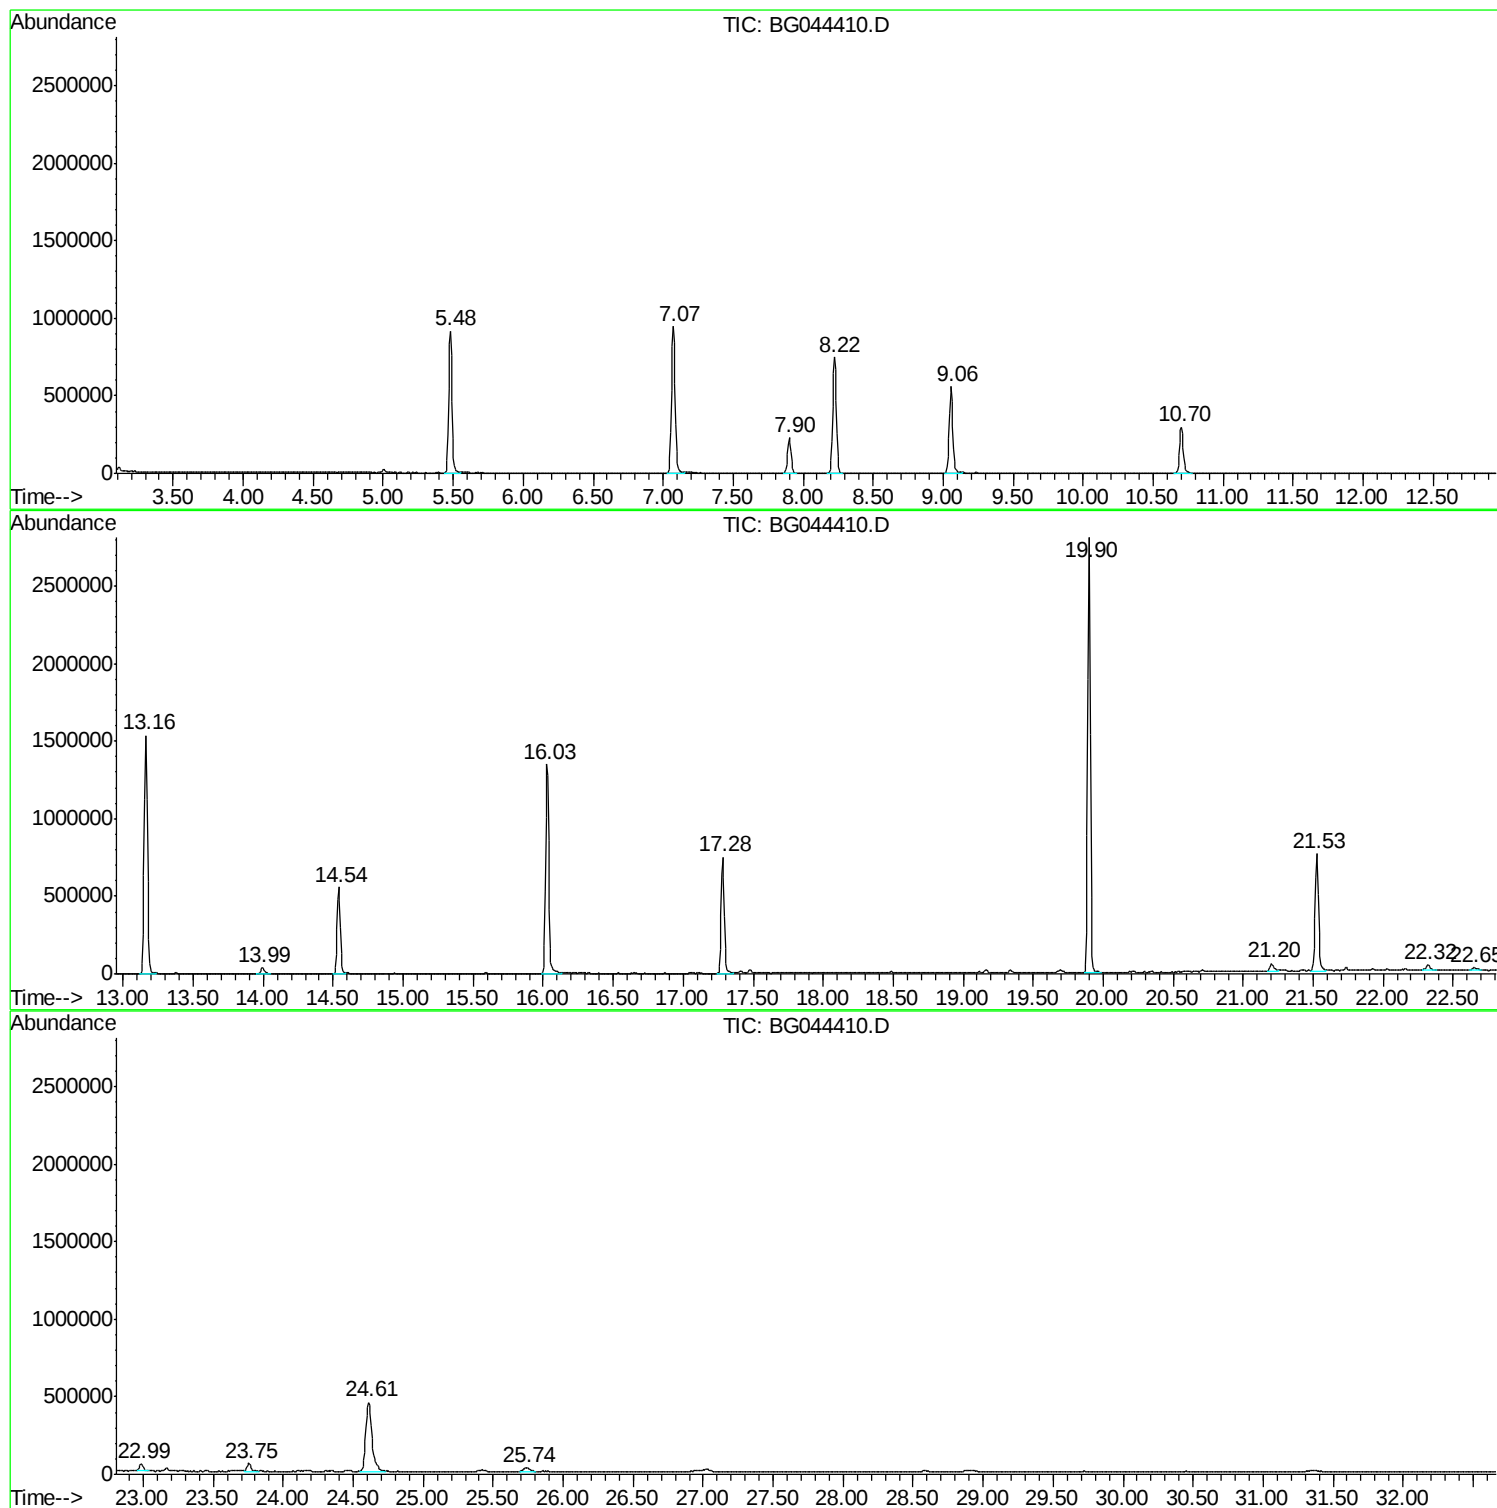

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021220\
Data File : BG044410.D
Acq On : 12 Feb 2020 15:51
Operator : CG/JU
Sample : L1491-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1E-(7.5-9.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021220\
Data File : BG044410.D
Acq On : 12 Feb 2020 15:51
Operator : CG/JU
Sample : L1491-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1E-(7.5-9.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc