


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021220\
 Data File : BG044404.D
 Acq On : 12 Feb 2020 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

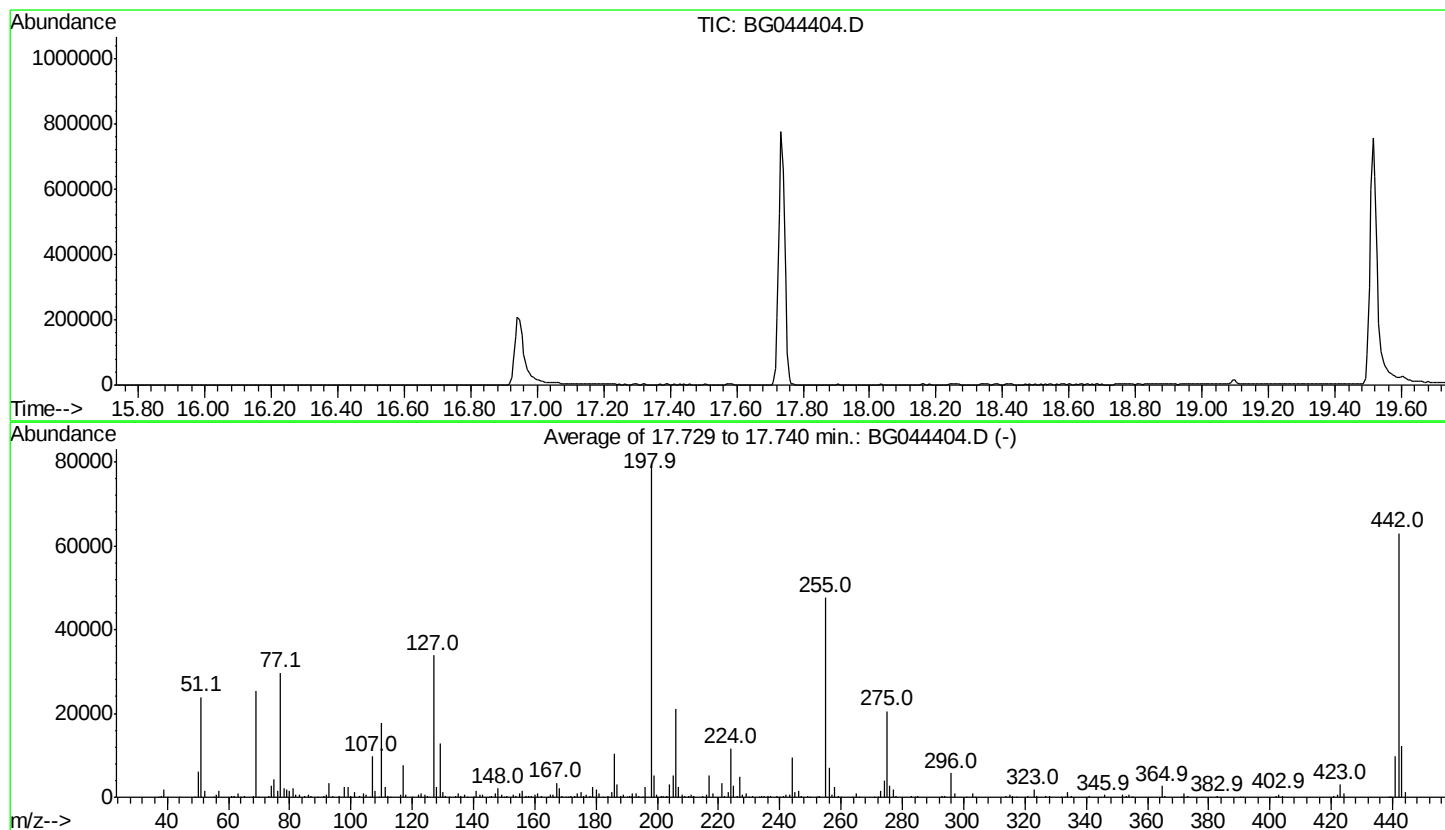

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	23938	PASS
68	69	0.00	2	0.8	192	PASS
69	198	0.00	100	31.9	25248	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	42.7	33802	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79160	PASS
199	198	5	9	6.6	5210	PASS
275	198	10	60	25.9	20540	PASS
365	198	1	100	3.4	2715	PASS
441	198	0.01	100	12.5	9886	PASS
442	198	50	100	79.6	62973	PASS
443	442	15	24	19.6	12323	PASS