

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021221\
 Data File : BG048147.D
 Acq On : 12 Feb 2021 13:40
 Operator : CG/JU
 Sample : PB134600BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK600

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.508	25	29	33	rBV2	15130	18688	1.09%	0.114%
2	3.731	66	67	70	rVB3	2299	1913	0.11%	0.012%
3	3.854	86	88	93	rVB4	2776	2853	0.17%	0.017%
4	3.919	95	99	114	rVV	163833	297077	17.35%	1.812%
5	4.031	116	118	121	rVV3	3812	3933	0.23%	0.024%
6	4.160	137	140	143	rVB2	2248	2867	0.17%	0.017%
7	4.189	143	145	150	rBV4	2072	3199	0.19%	0.020%
8	4.266	154	158	161	rBV4	1514	2245	0.13%	0.014%
9	4.318	166	167	169	rBV	2179	1916	0.11%	0.012%
10	4.824	251	253	257	rVB3	2142	2184	0.13%	0.013%
11	5.194	315	316	319	rBV	2828	2464	0.14%	0.015%
12	5.270	326	329	332	rBV3	1478	1836	0.11%	0.011%
13	5.635	389	391	394	rVB4	2007	2255	0.13%	0.014%
14	5.670	394	397	398	rBV2	1779	1956	0.11%	0.012%
15	6.216	488	490	496	rVB4	1502	2121	0.12%	0.013%
16	6.269	496	499	501	rBV3	1256	1746	0.10%	0.011%
17	7.244	659	665	674	rVV	225364	399113	23.30%	2.434%
18	7.421	686	695	703	rBV	169784	280153	16.36%	1.709%
19	7.626	721	730	741	rBV	222416	390015	22.77%	2.379%
20	7.715	743	745	750	rVB	1372	1933	0.11%	0.012%
21	7.761	750	753	756	rBV2	1652	1801	0.11%	0.011%
22	7.938	781	783	790	rVB3	1183	2030	0.12%	0.012%
23	8.102	804	811	819	rVB	177341	290880	16.98%	1.774%
24	8.796	922	929	938	rBV2	266400	470926	27.50%	2.872%
25	9.260	1001	1008	1017	rVB	212809	378893	22.12%	2.311%
26	9.612	1066	1068	1071	rVB2	1753	1723	0.10%	0.011%
27	9.988	1124	1132	1142	rBV	189653	342819	20.02%	2.091%
28	10.529	1214	1224	1232	rBV	263303	490668	28.65%	2.993%
29	10.582	1232	1233	1239	rVB4	2350	3196	0.19%	0.019%
30	10.711	1251	1255	1258	rVV2	1472	1950	0.11%	0.012%
31	10.917	1281	1290	1299	rVB	228312	398437	23.26%	2.430%
32	11.040	1302	1311	1322	rBV	259182	483526	28.23%	2.949%
33	12.497	1551	1559	1565	rVB5	4007	9011	0.53%	0.055%
34	13.913	1794	1800	1802	rBV3	1209	1834	0.11%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021221\
 Data File : BG048147.D
 Acq On : 12 Feb 2021 13:40
 Operator : CG/JU
 Sample : PB134600BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK600

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
 Title : SVOA CALIBRATION

35	14.125	1829	1836	1845	rBV	573614	828799	48.39%	5.055%
36	14.418	1878	1886	1893	rBV	600547	922207	53.84%	5.625%
37	14.724	1930	1938	1946	rVB	385712	619396	36.16%	3.778%
38	14.900	1960	1968	1987	rBV	236869	422007	24.64%	2.574%
39	15.717	2099	2107	2114	rBV	750271	1169447	68.28%	7.133%
40	15.823	2119	2125	2138	rVV	246558	396029	23.12%	2.415%
41	15.952	2142	2147	2155	rVB6	10918	17893	1.04%	0.109%
42	16.163	2179	2183	2185	rBV2	2173	2364	0.14%	0.014%
43	16.387	2217	2221	2226	rBV3	1125	2202	0.13%	0.013%
44	16.498	2235	2240	2244	rBV4	3499	4164	0.24%	0.025%
45	17.004	2324	2326	2330	rBV2	1421	1826	0.11%	0.011%
46	17.151	2346	2351	2352	rBV2	2417	2969	0.17%	0.018%
47	17.203	2358	2360	2365	rBV3	1819	2504	0.15%	0.015%
48	17.244	2365	2367	2371	rBV4	2805	3923	0.23%	0.024%
49	17.468	2398	2405	2412	rBV	547634	818654	47.80%	4.993%
50	17.568	2415	2422	2429	rVV2	920195	1354449	79.08%	8.261%
51	17.644	2432	2435	2437	rVB3	2467	2527	0.15%	0.015%
52	17.709	2443	2446	2449	rBV3	2141	2446	0.14%	0.015%
53	17.785	2455	2459	2460	rBV3	1591	2124	0.12%	0.013%
54	17.932	2481	2484	2486	rVB3	1849	1725	0.10%	0.011%
55	17.973	2486	2491	2494	rBV2	2328	3420	0.20%	0.021%
56	18.026	2496	2500	2502	rBV3	2110	3676	0.21%	0.022%
57	18.214	2528	2532	2536	rVB6	2239	2871	0.17%	0.018%
58	18.279	2541	2543	2544	rBV2	2376	1761	0.10%	0.011%
59	18.326	2547	2551	2553	rBV3	1478	2279	0.13%	0.014%
60	18.490	2576	2579	2580	rVB	2693	2638	0.15%	0.016%
61	18.649	2603	2606	2608	rBV3	2355	2622	0.15%	0.016%
62	18.802	2630	2632	2635	rBV4	2284	2612	0.15%	0.016%
63	18.972	2658	2661	2662	rBV3	3124	2472	0.14%	0.015%
64	19.048	2673	2674	2676	rBV2	1850	1811	0.11%	0.011%
65	19.383	2729	2731	2732	rBV2	2273	1746	0.10%	0.011%
66	19.483	2744	2748	2751	rBV2	13014	17815	1.04%	0.109%
67	19.565	2761	2762	2764	rBV2	2867	2040	0.12%	0.012%
68	19.589	2764	2766	2767	rVV	2137	1713	0.10%	0.010%
69	19.677	2780	2781	2783	rBV2	3020	1714	0.10%	0.010%
70	19.736	2787	2791	2794	rVV3	9843	12725	0.74%	0.078%
71	19.847	2803	2810	2816	rBV	1181714	1712709	100.00%	10.446%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021221\
 Data File : BG048147.D
 Acq On : 12 Feb 2021 13:40
 Operator : CG/JU
 Sample : PB134600BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK600

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
 Title : SVOA CALIBRATION

72	19.971	2829	2831	2833	rBV3	4008	2526	0.15%	0.015%
73	20.212	2867	2872	2874	rBV6	7977	13892	0.81%	0.085%
74	20.646	2944	2946	2947	rBV2	5846	3952	0.23%	0.024%
75	21.457	3080	3084	3088	rBV2	23067	34943	2.04%	0.213%
76	21.739	3125	3132	3141	rVB	566933	957242	55.89%	5.838%
77	22.550	3266	3270	3274	rBV6	13096	20028	1.17%	0.122%
78	23.249	3387	3389	3394	rVB6	17032	24253	1.42%	0.148%
79	24.072	3525	3529	3534	rVB4	23058	45326	2.65%	0.276%
80	24.783	3639	3650	3662	rBV2	568391	1568510	91.58%	9.567%
81	25.006	3678	3688	3701	rVB2	328205	998897	58.32%	6.092%
82	26.193	3885	3890	3898	rVB7	28052	73682	4.30%	0.449%


Sum of corrected areas: 16395691

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021221\
Data File : BG048147.D
Acq On : 12 Feb 2021 13:40
Operator : CG/JU
Sample : PB134600BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK600

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

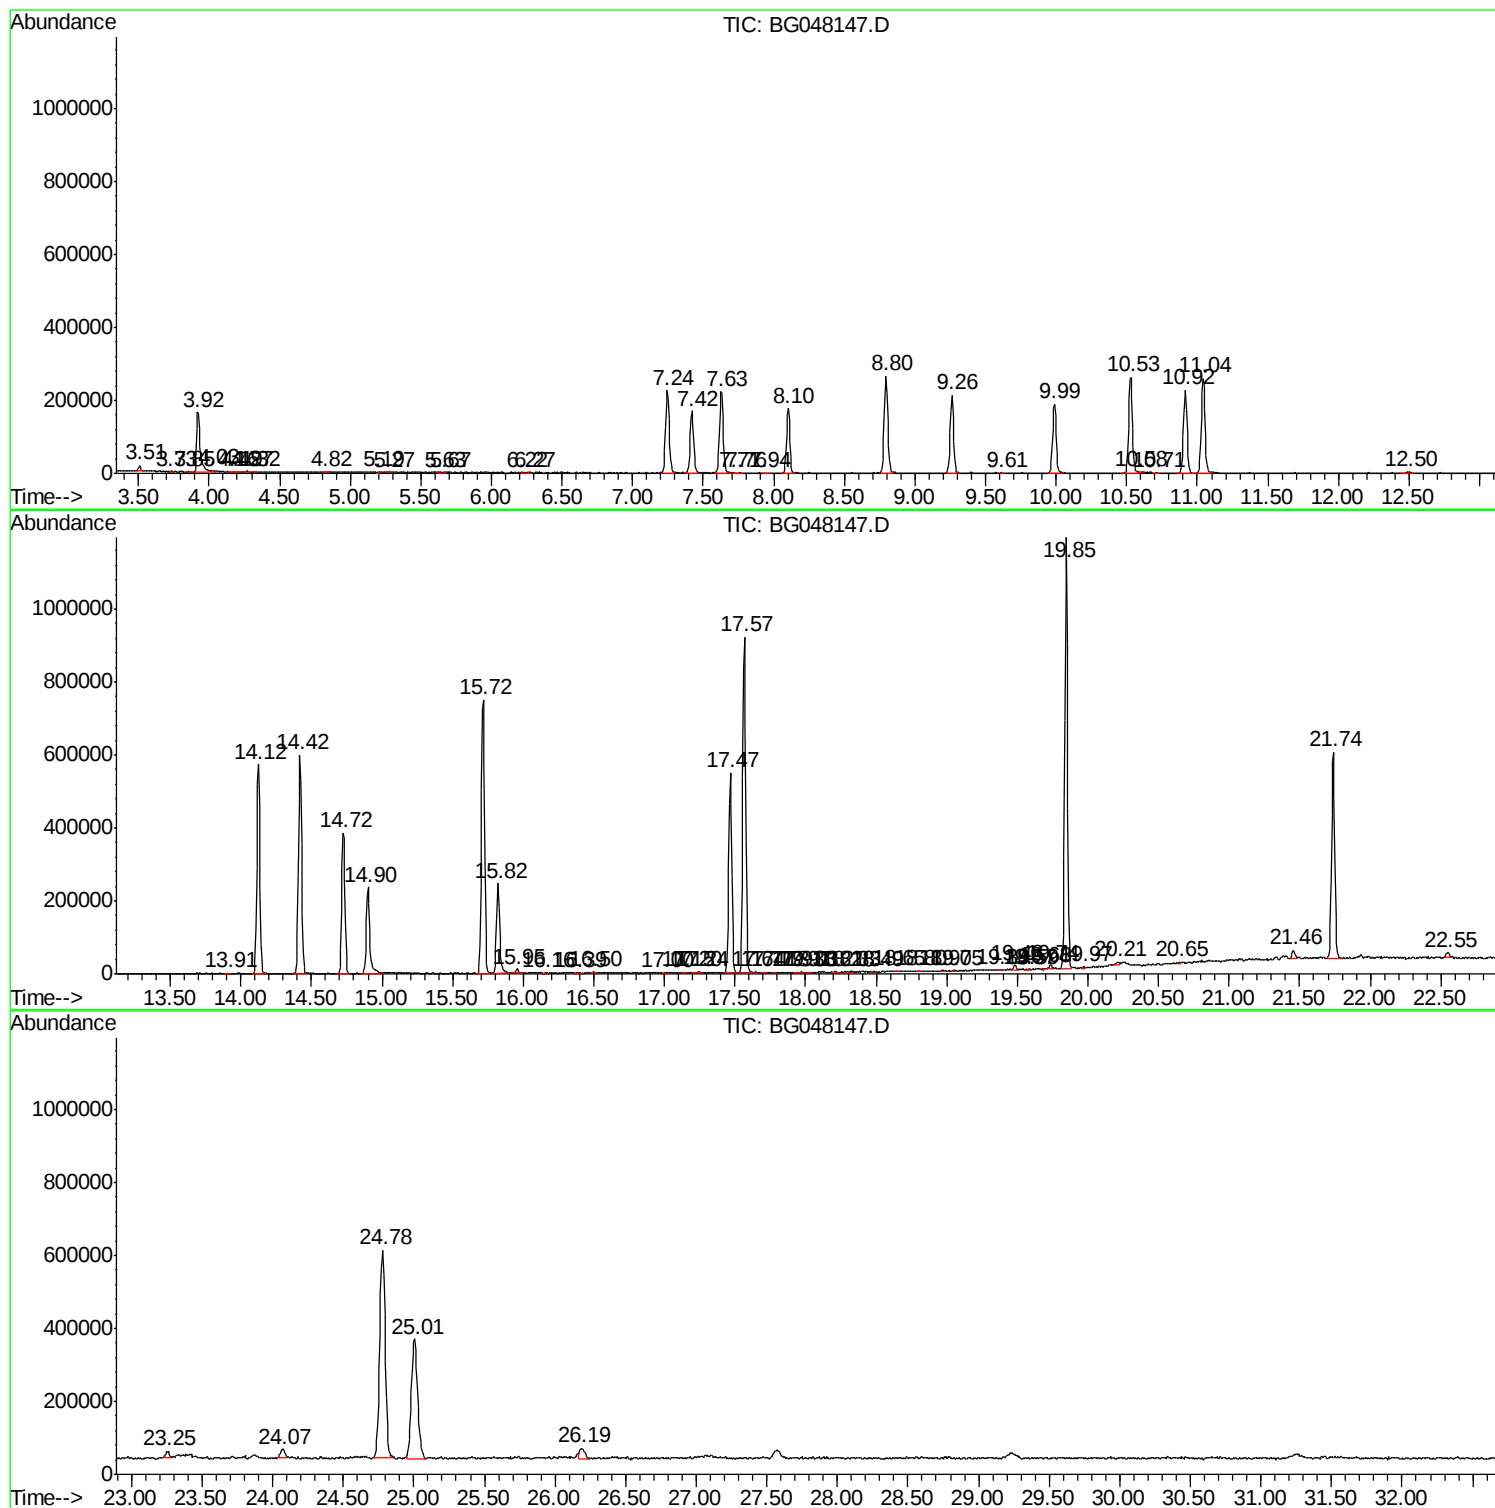

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021221\
Data File : BG048147.D
Acq On : 12 Feb 2021 13:40
Operator : CG/JU
Sample : PB134600BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK600

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021221\
Data File : BG048147.D
Acq On : 12 Feb 2021 13:40
Operator : CG/JU
Sample : PB134600BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK600

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG012921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc