

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021317\
 Data File : BG025841.D
 Acq On : 13 Feb 2017 11:13
 Operator : SJ/MA
 Sample : I1746-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0FK2

Quant Time: Feb 13 13:38:14 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG021017MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 10 22:04:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	87223	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	427489	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	311921	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.42	188	684173	20.00	ng/ul	0.00
77) Chrysene-d12	21.68	240	700612	20.00	ng/ul	0.00
85) Perylene-d12	24.88	264	675080	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.52	96	9976	5.11	ng/uL	0.00
5) Phenol-d5	7.23	99	49784	6.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	133130	26.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	136556	22.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.78	113	100504	14.78	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	79008	28.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	90530	30.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.50	165	174822	27.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.02	131	16510	2.04	ng/ul	0.00
43) Dimethylphthalate-d6	14.09	166	721113	31.55	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	808827	30.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	33246	7.61	ng/ul	0.00
57) Fluorene-d10	15.68	176	634408	31.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.78	200	108525	31.09	ng/ul	0.00
70) Anthracene-d10	17.52	188	1035388	33.36	ng/ul	0.00
78) Pyrene-d10	19.79	212	1134878	33.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.67	264	1049031	34.98	ng/ul	0.00


Target Compounds						Ovalue
56) Diethylphthalate	15.49	149	72944	3.18	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021317\
Data File : BG025841.D
Acq On : 13 Feb 2017 11:13
Operator : SJ/MA
Sample : I1746-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0FK2

Quant Time: Feb 13 13:38:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG021017MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 10 22:04:56 2017
Response via : Initial Calibration

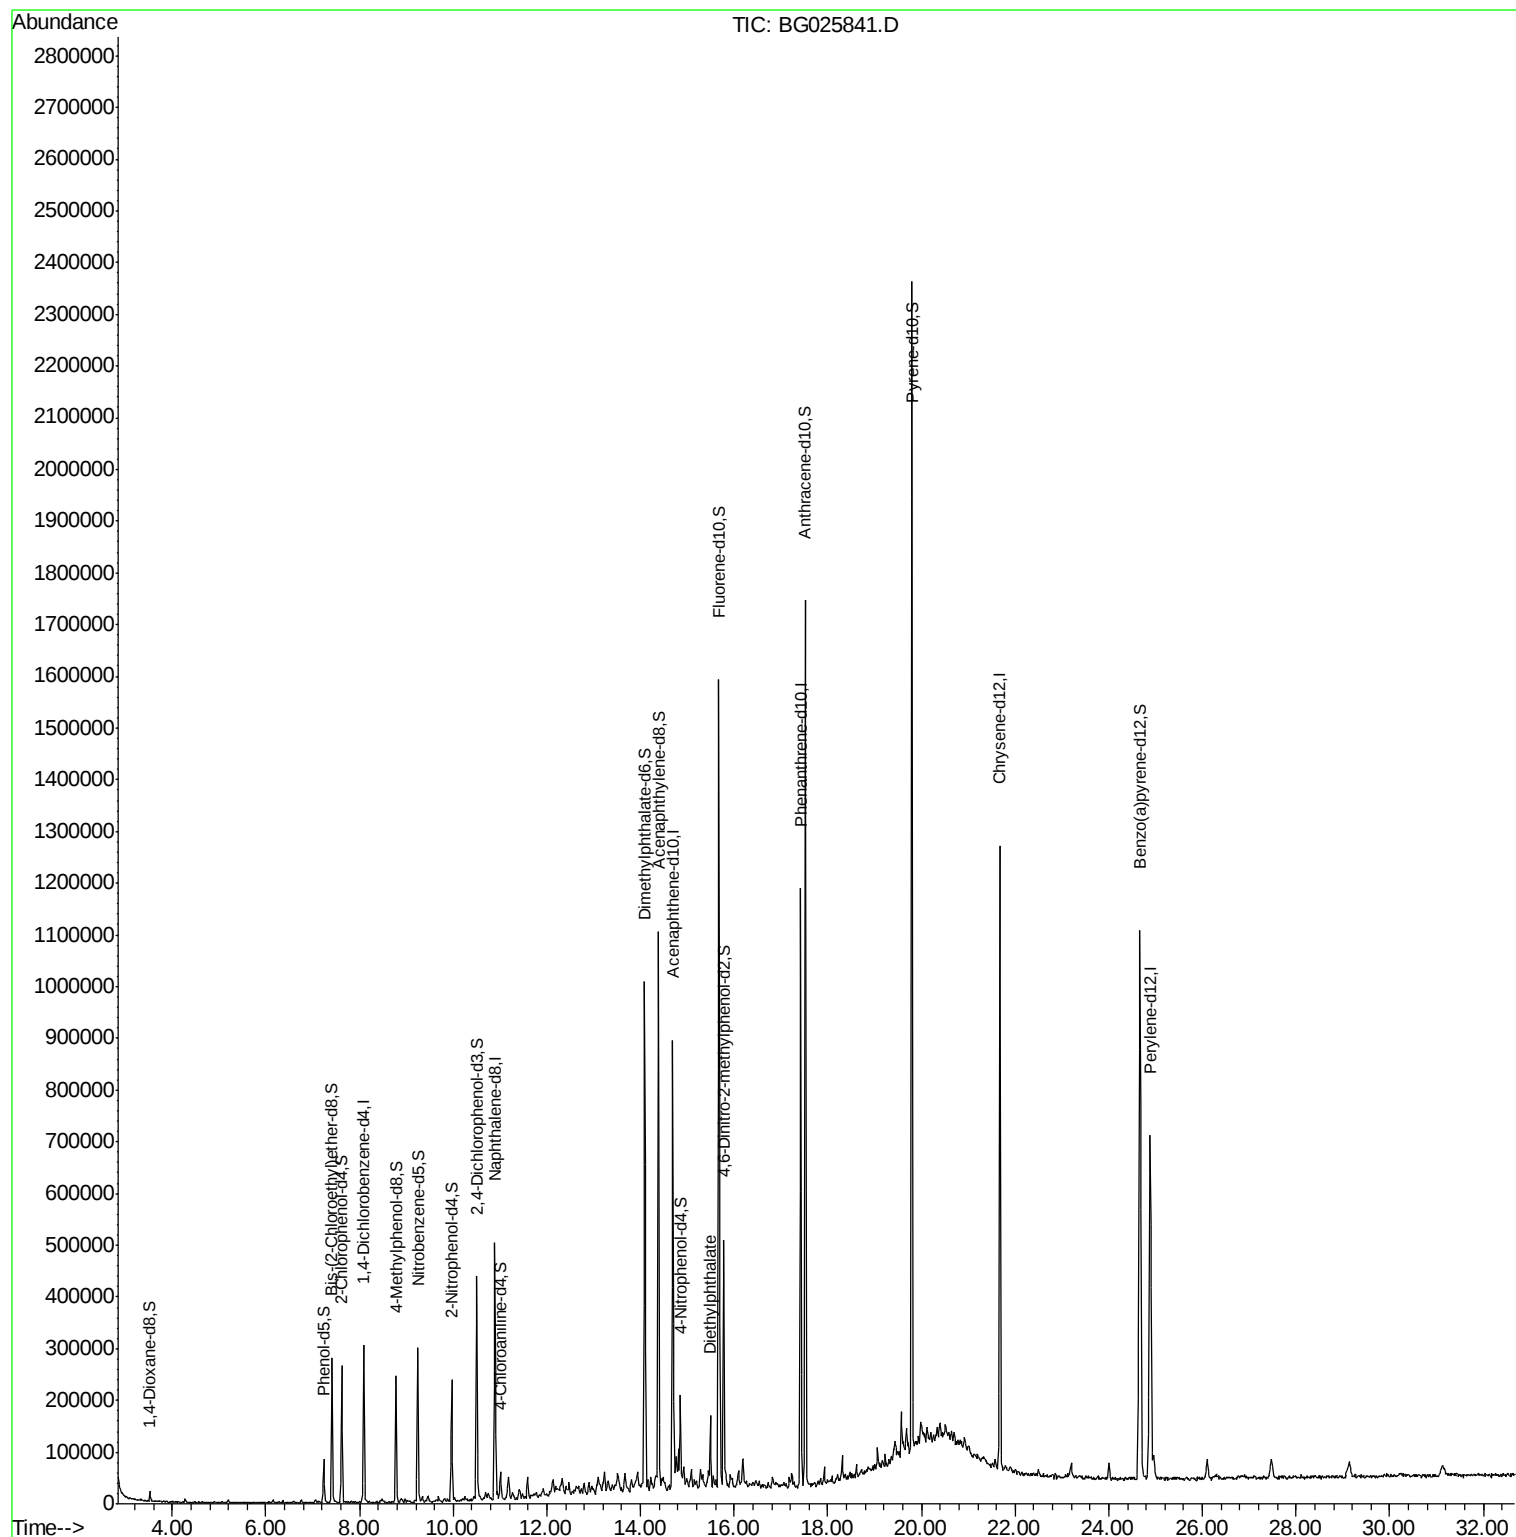


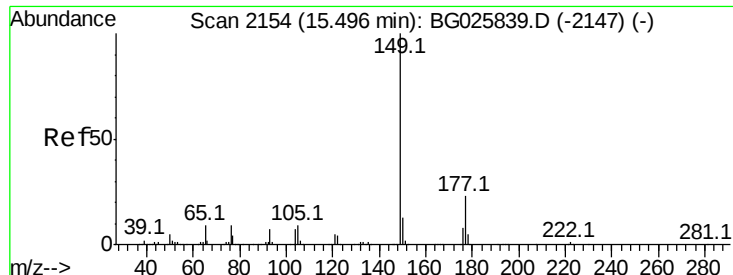

#56
 Diethylphthalate
 Concen: 3.18 ng/ul
 RT: 15.49 min Scan# 2154
 Delta R.T. -0.01 min
 Lab File: BG025841.D
 Acq: 13 Feb 2017 11:13

Instrument :
 BNA_G
 ClientSampleId :
 H0FK2

Tot Ion	Ratio	Lower	Upper
149	100		
177	23.5	17.4	26.2
150	12.1	10.0	15.0

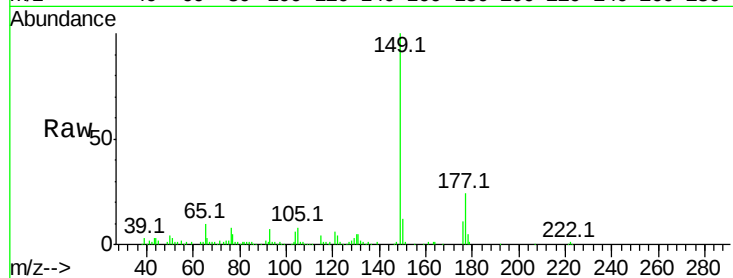

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

