
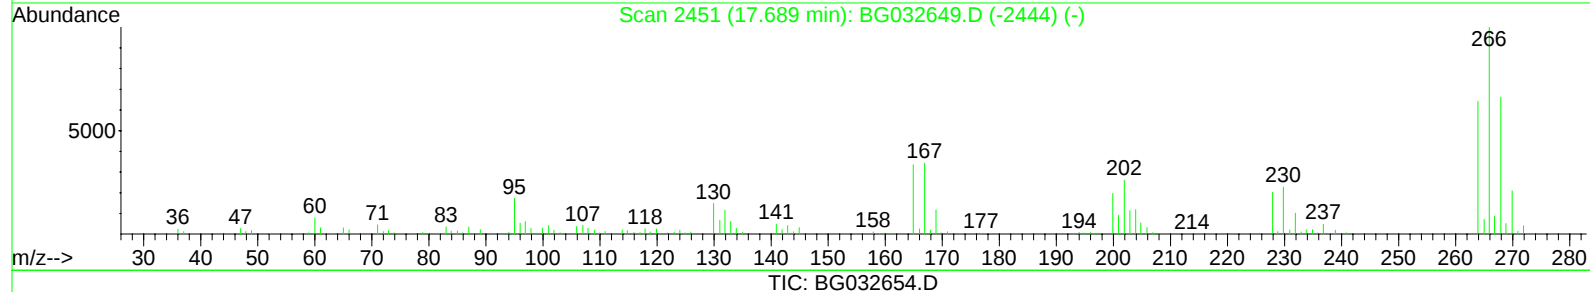
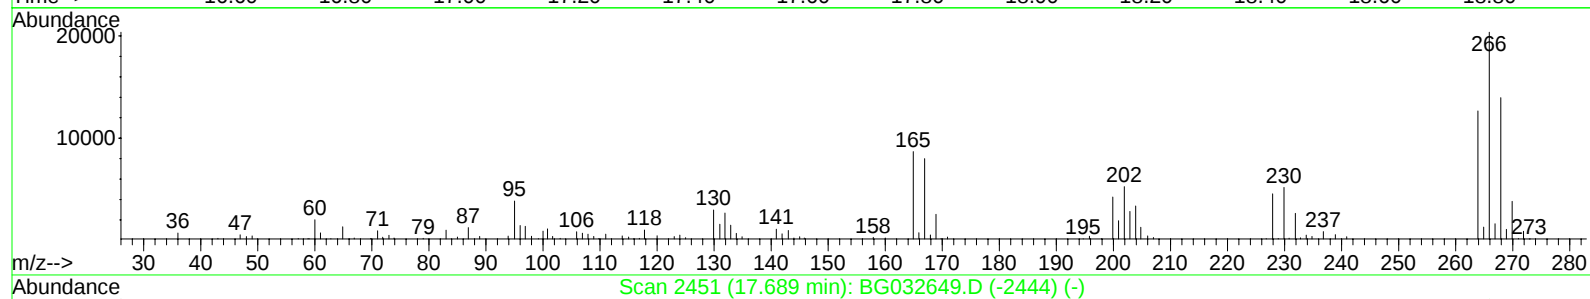


Data Path : Z:\HPCHEM1\BNA G\Data\BG021318\
Data File : BG032654.D
Acq On : 13 Feb 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 05:54:26 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

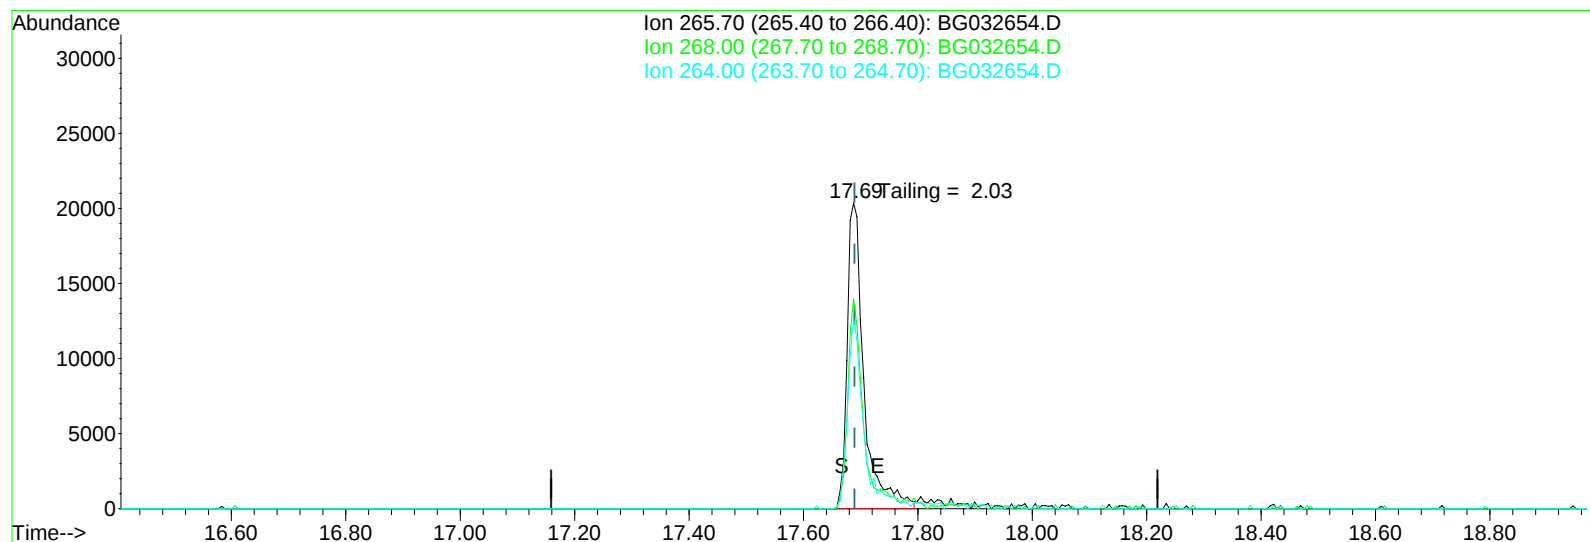

(69) Pentachlorophenol (C)




17.688min (-0.001) 15495.27ng

response 41557

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.51
264.00	62.00	62.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG021318\
 Data File : BG032654.D
 Acq On : 13 Feb 2018 11:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 05:54:26 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 12 18:08:01 2018
 Response via : Initial Calibration

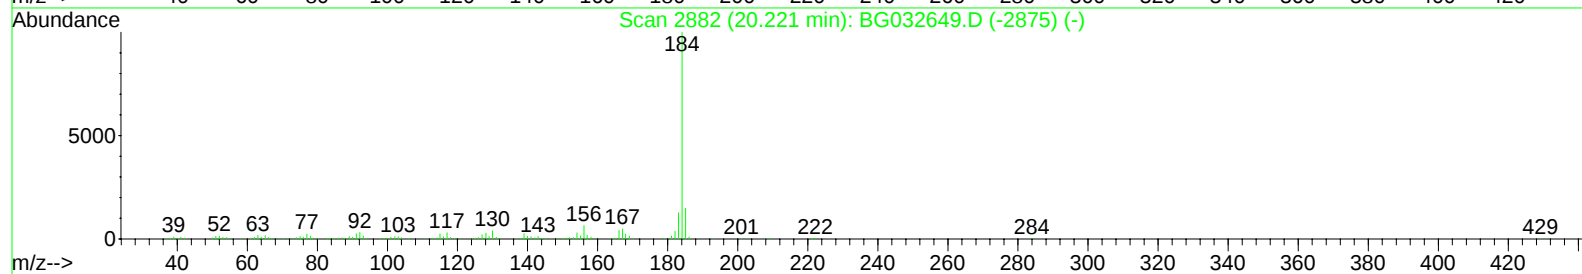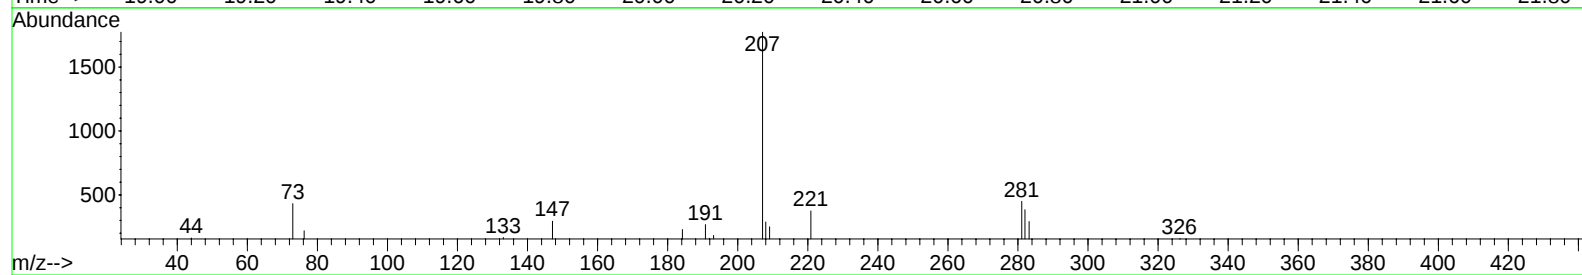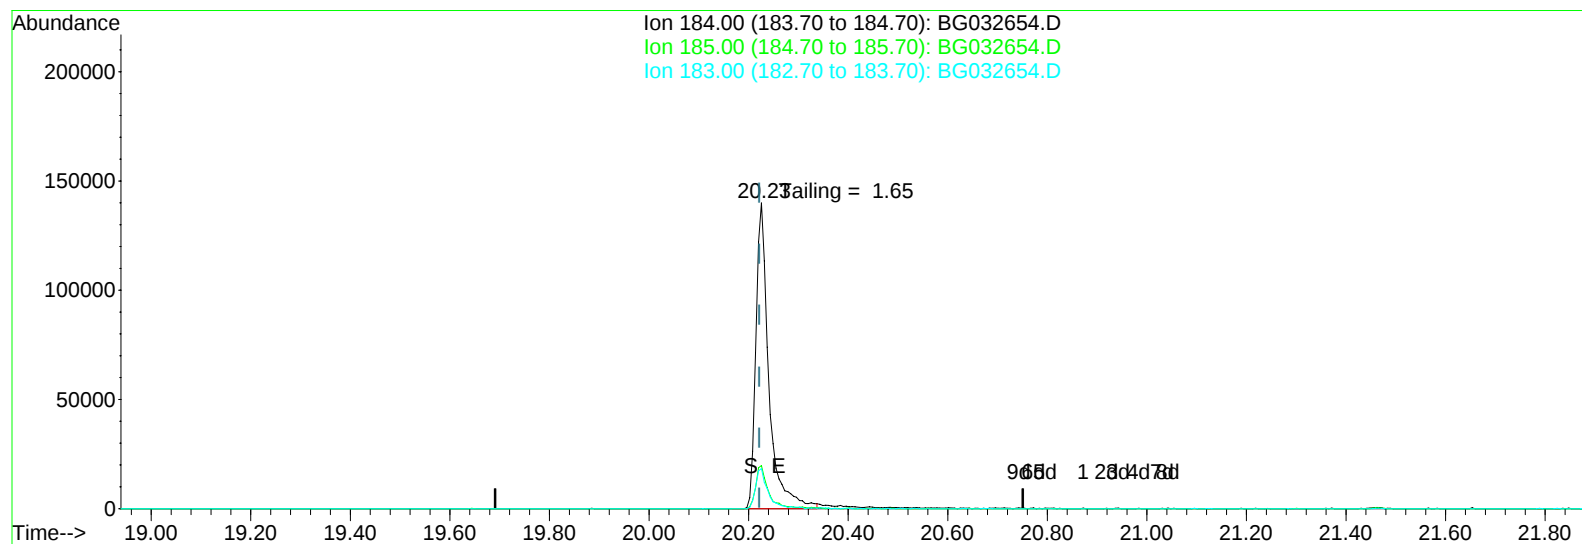

TIC: BG032654.D

(76) Benzidine

20.872min (+0.651) 55.48ng

response 81

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00