
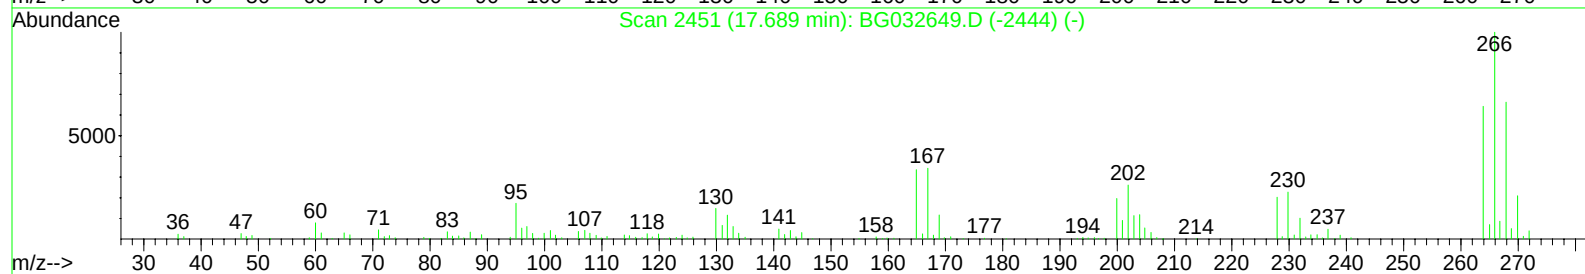
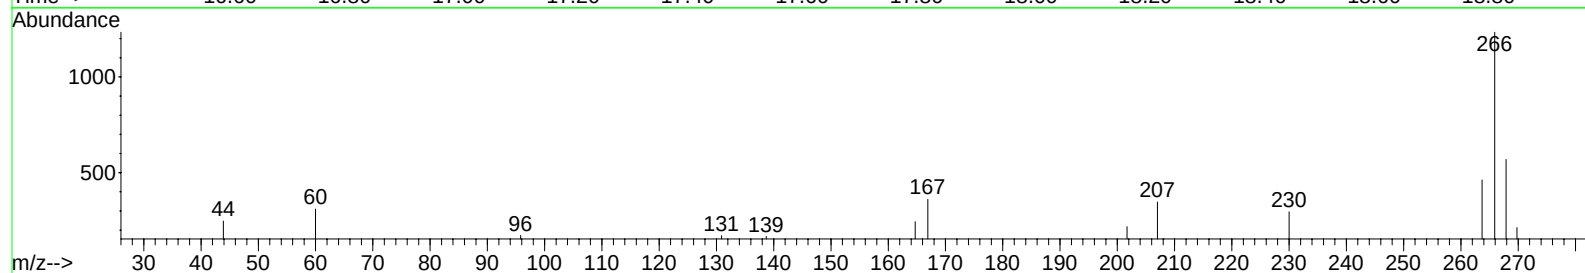


Data Path : Z:\HPCHEM1\BNA G\Data\BG021318\
Data File : BG032673.D
Acq On : 13 Feb 2018 23:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 05:55:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

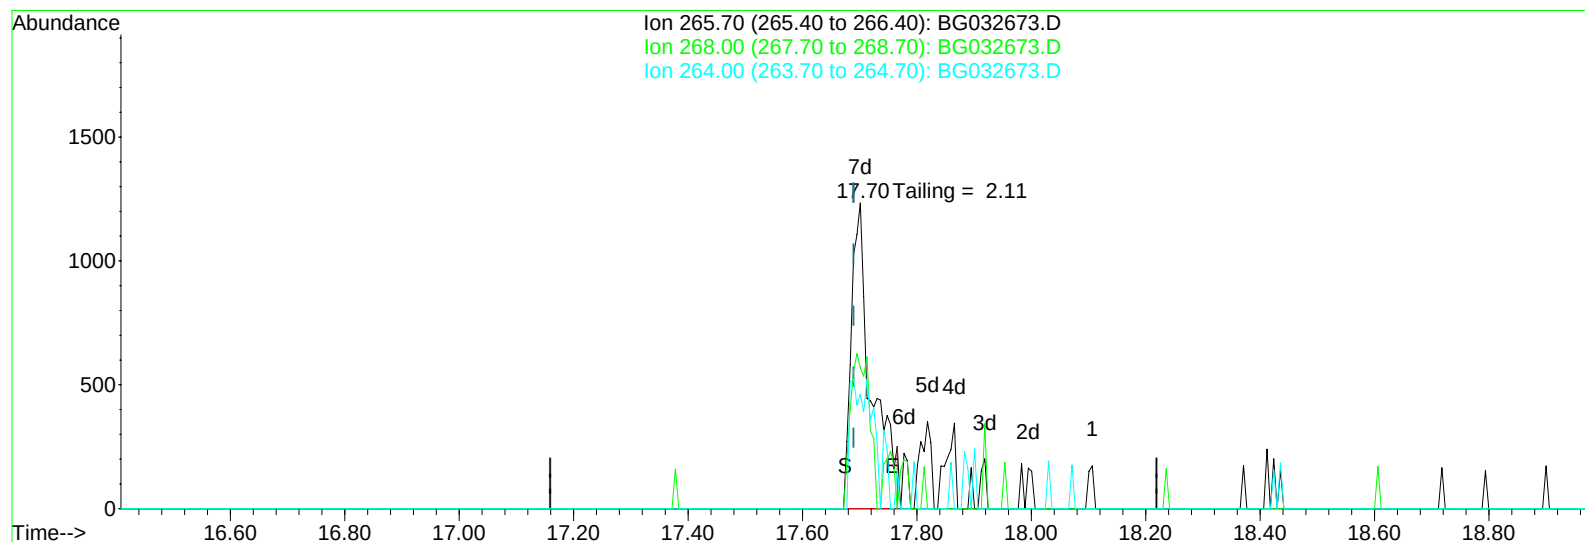

TIC: BG032673.D

(69) Pentachlorophenol (C)




17.701min (+0.012) 838.92ng m

response 3142

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	46.11#
264.00	62.00	37.44#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG021318\
Data File : BG032673.D
Acq On : 13 Feb 2018 23:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 05:55:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

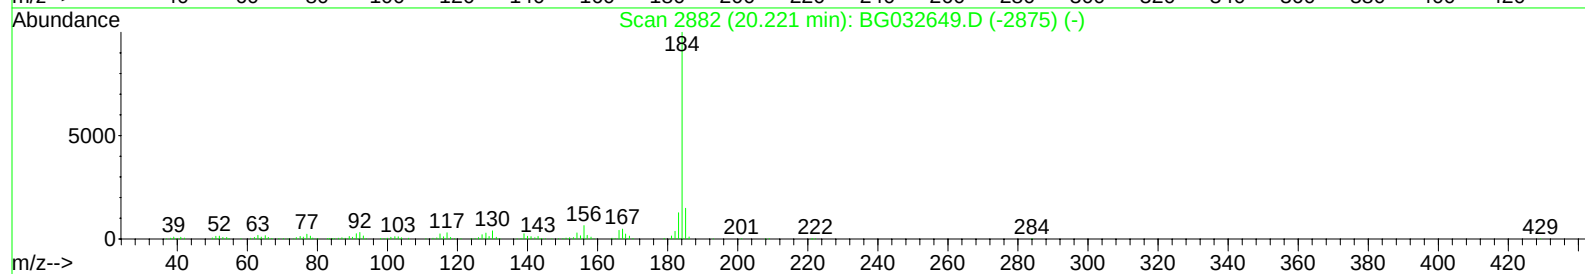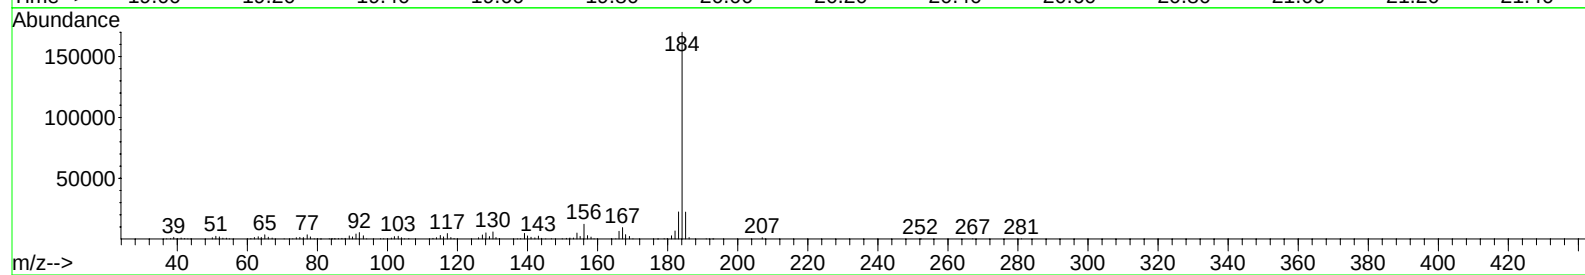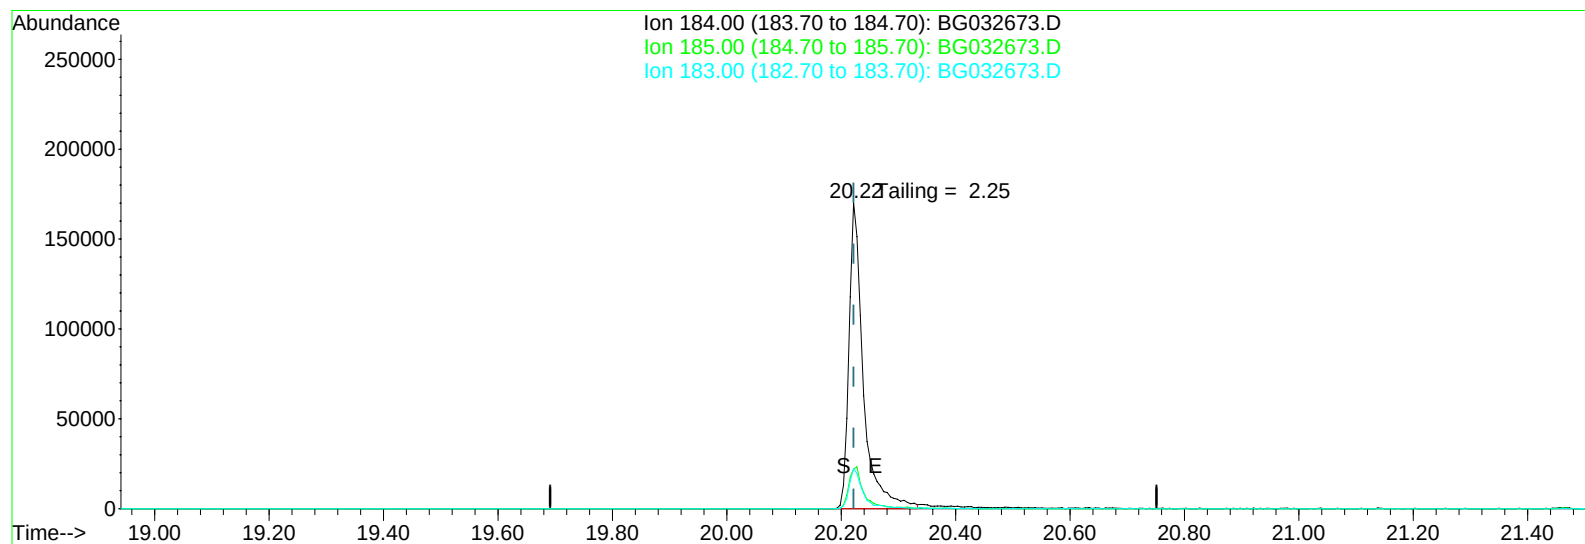

TIC: BG032673.D

(76) Benzidine

20.222min (+0.000) 0.00ng

response 300493

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.03
183.00	13.30	13.09
0.00	0.00	0.00