


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021318\
 Data File : BG032654.D
 Acq On : 13 Feb 2018 11:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 12 18:08:01 2018

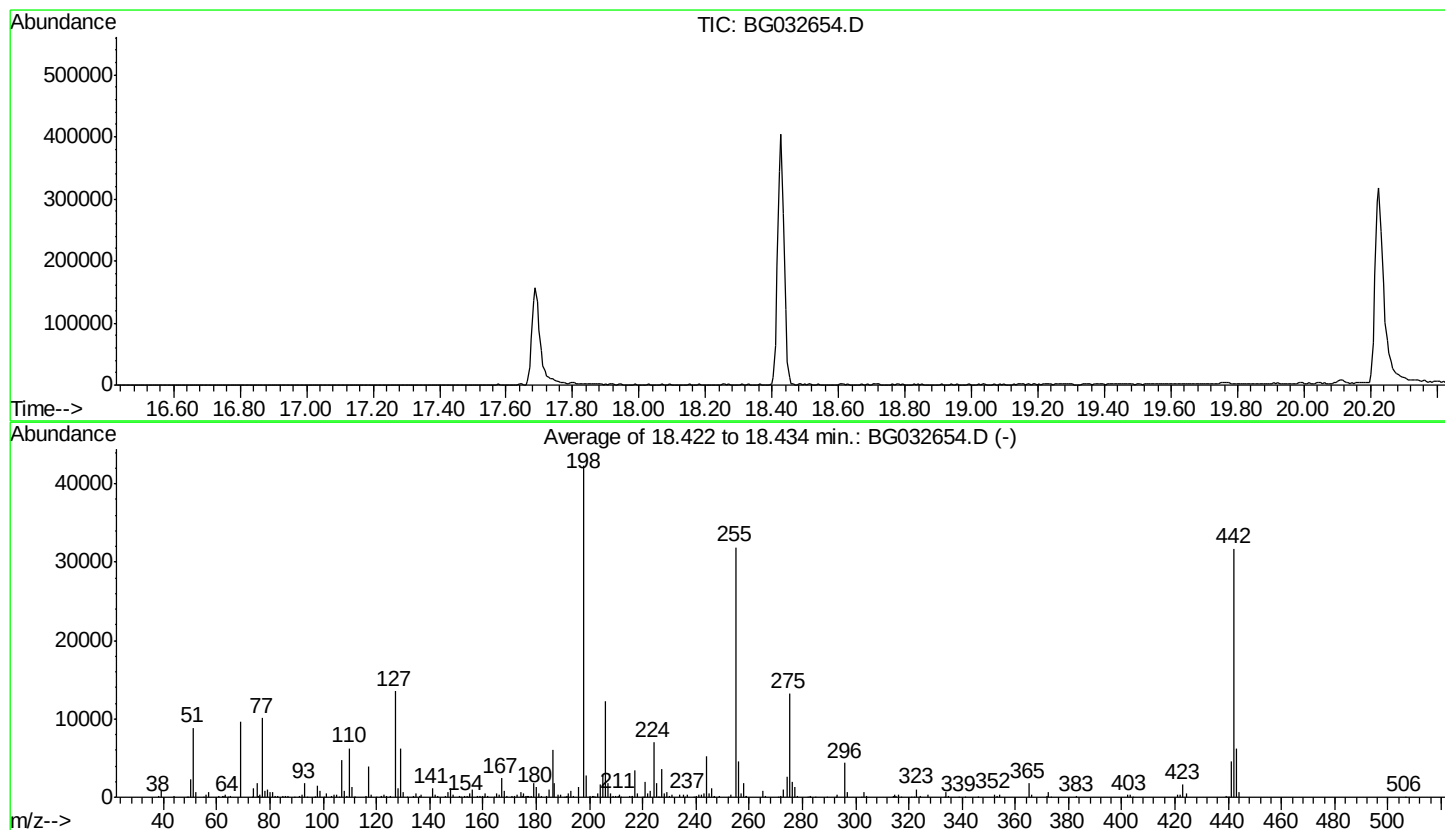

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	8891	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.9	9687	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.9	13482	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42298	PASS
199	198	5	9	6.7	2851	PASS
275	198	10	60	31.2	13199	PASS
365	198	1	100	4.1	1744	PASS
441	442	0.01	24	14.6	4646	PASS
442	198	50	100	75.0	31736	PASS
443	442	15	24	19.8	6286	PASS