


Data Path : Z:\HPCHEM1\BNA G\Data\BG021318\
 Data File : BG032673.D
 Acq On : 13 Feb 2018 23:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 12 18:08:01 2018

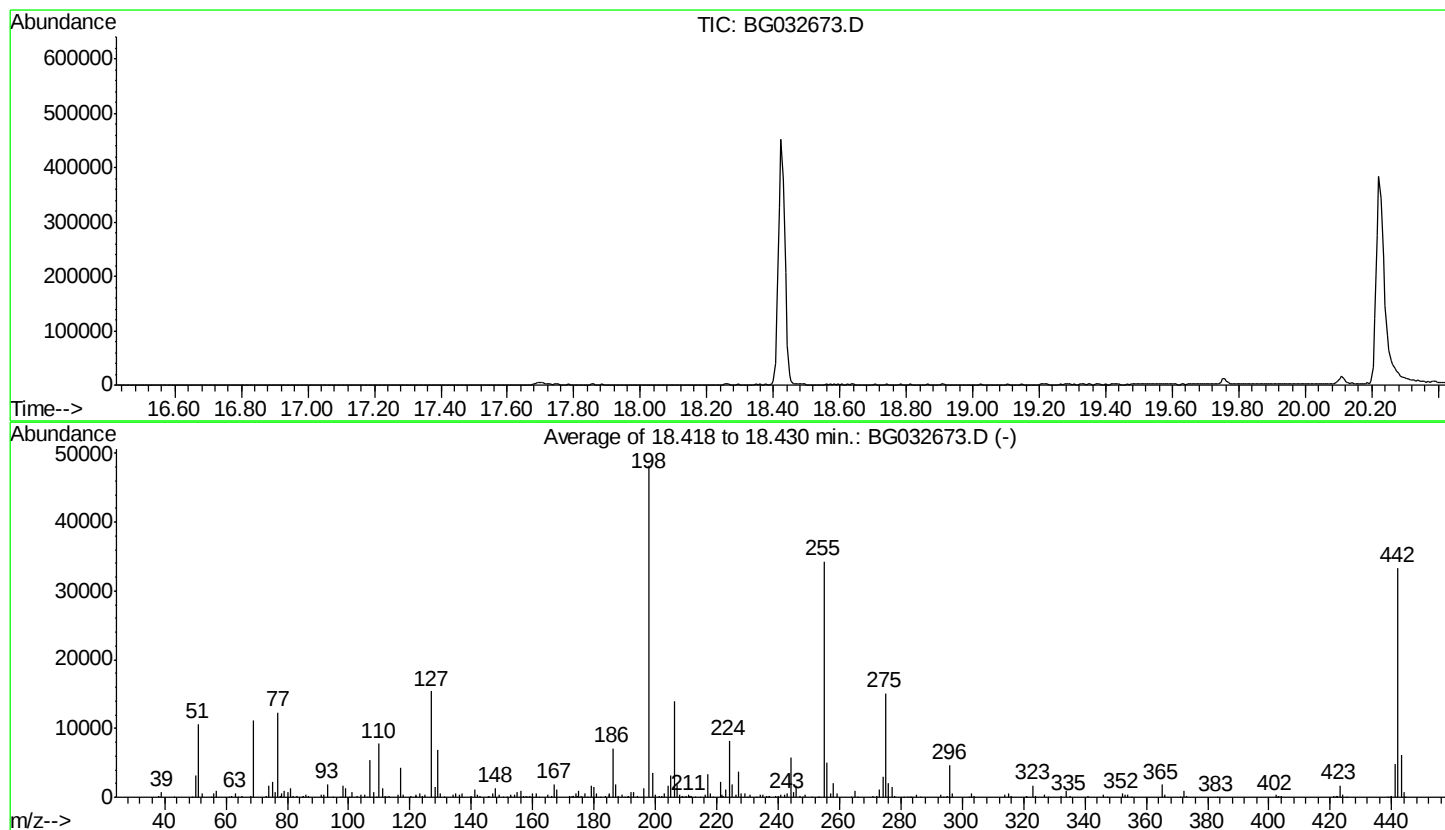

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	10701	PASS
68	69	0.00	2	1.2	133	PASS
69	198	0.00	100	23.3	11211	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.9	15394	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48189	PASS
199	198	5	9	7.4	3578	PASS
275	198	10	60	31.4	15146	PASS
365	198	1	100	3.9	1860	PASS
441	442	0.01	24	14.7	4896	PASS
442	198	50	100	69.2	33333	PASS
443	442	15	24	18.2	6064	PASS