
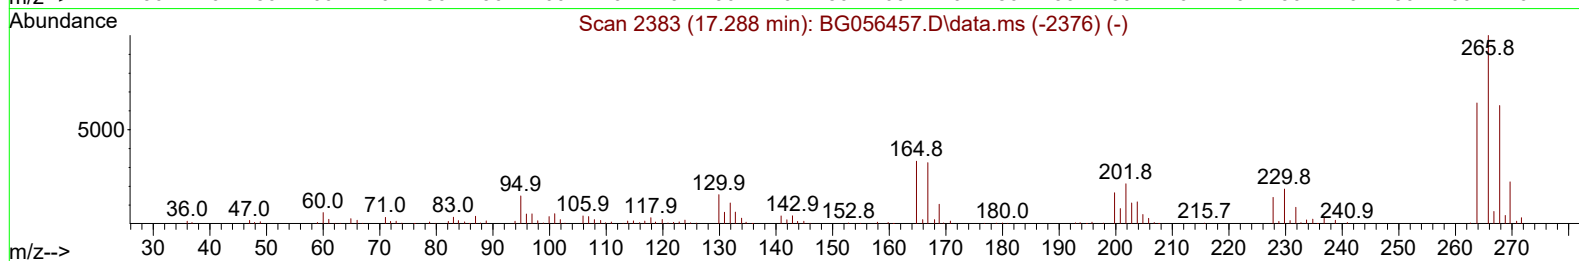
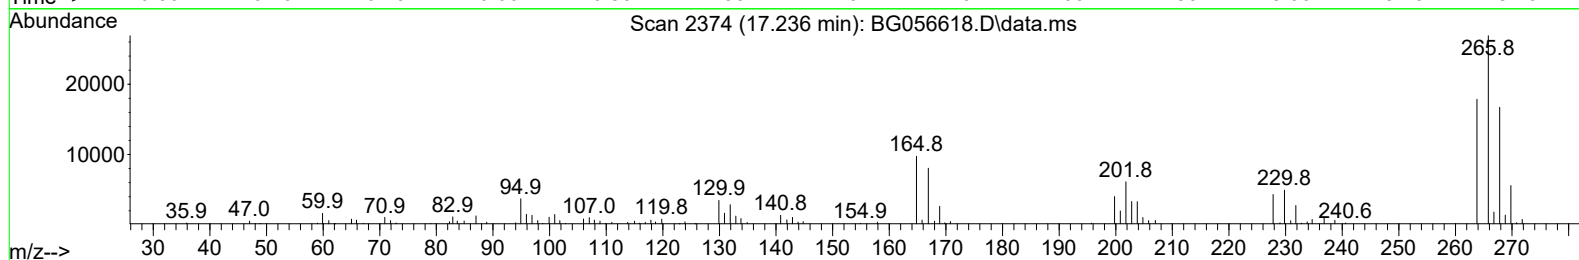


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021323\
Data File : BG056618.D
Acq On : 13 Feb 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:08:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

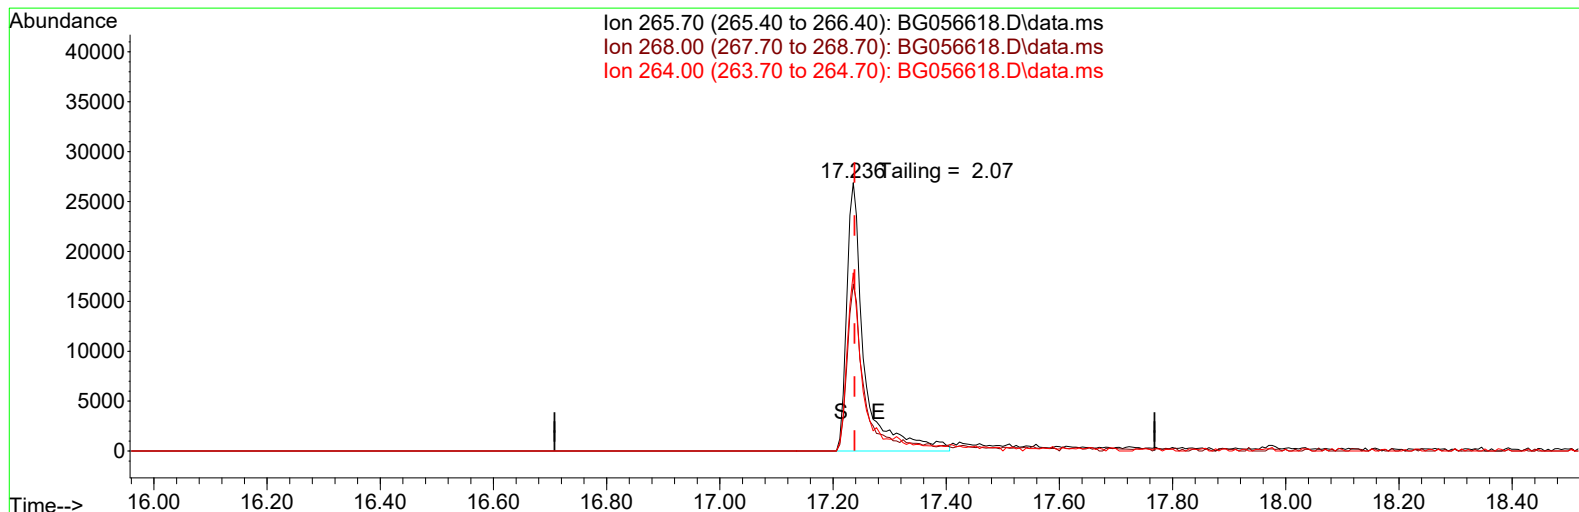

TIC: BG056618.D\data.ms

(70) Pentachlorophenol (C)




17.236min (-0.002) 14508.14 ng

response 56796

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.20
264.00	64.20	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021323\
Data File : BG056618.D
Acq On : 13 Feb 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:08:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

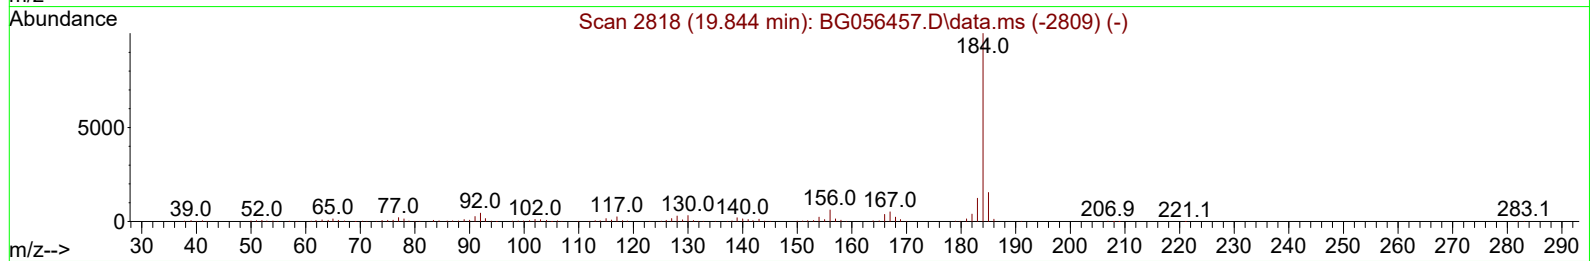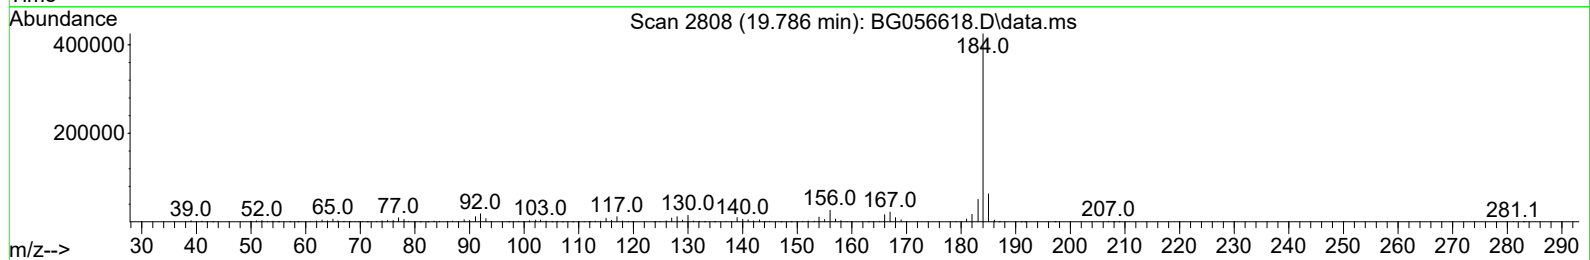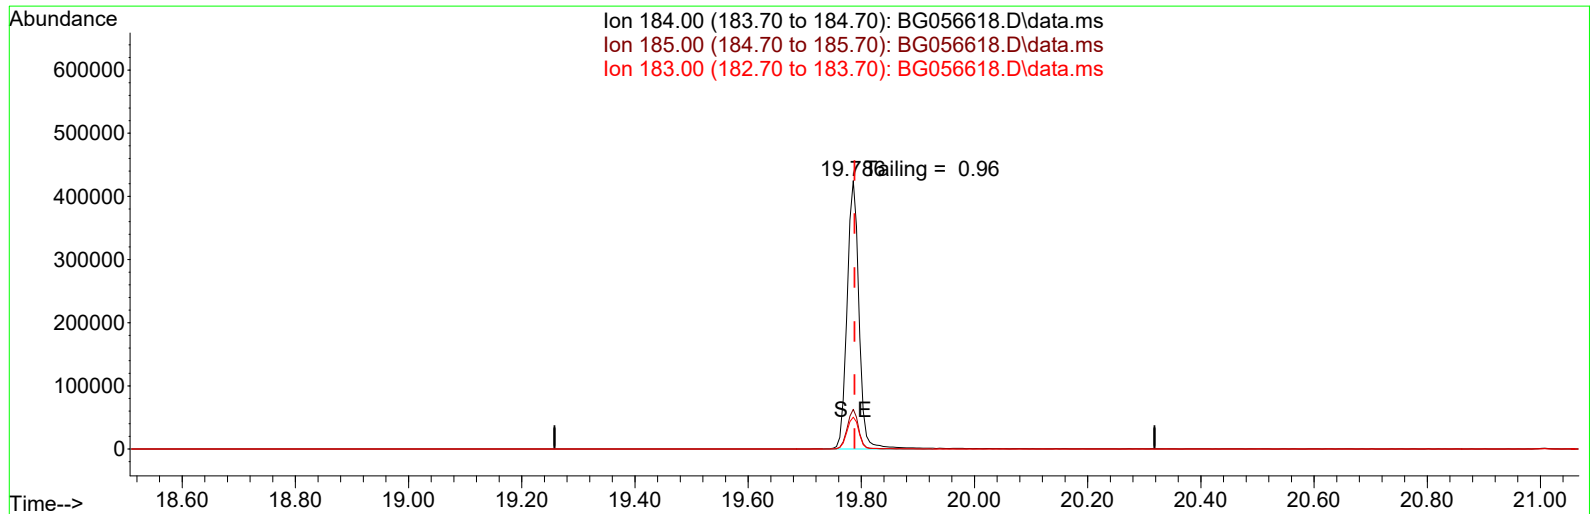

TIC: BG056618.D\data.ms

(77) Benzidine**19.786min (-0.002) 155856.88 ng****response 624216**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.82
183.00	12.30	11.91
0.00	0.00	0.00