
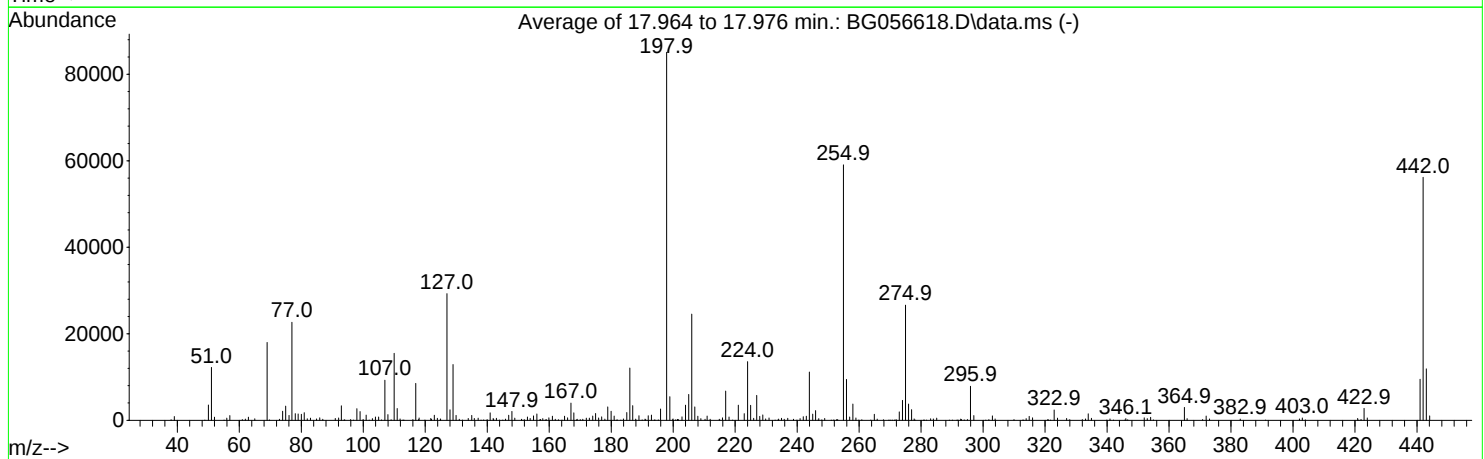


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021323\
Data File : BG056618.D
Acq On : 13 Feb 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 10 22:46:08 2023

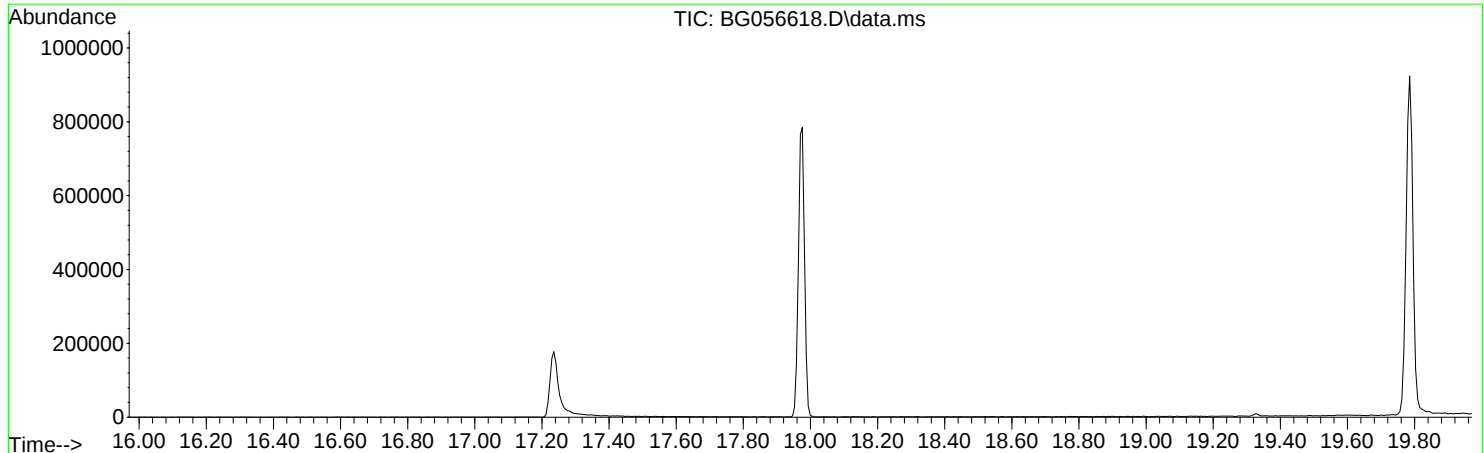




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.4	12226	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.2	17992	PASS
70	69	0.00	2	0.6	112	PASS
127	198	10	80	34.4	29275	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85053	PASS
199	198	5	9	6.4	5475	PASS
275	198	10	60	31.3	26626	PASS
365	198	1	100	3.5	2964	PASS
441	198	0.01	100	11.2	9491	PASS
442	442	50	100	100.0	56165	PASS
443	442	15	24	21.2	11906	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021323\
 Data File : BG056618.D
 Acq On : 13 Feb 2023 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 14 04:08:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 10 22:46:08 2023
 Response via : Initial Calibration

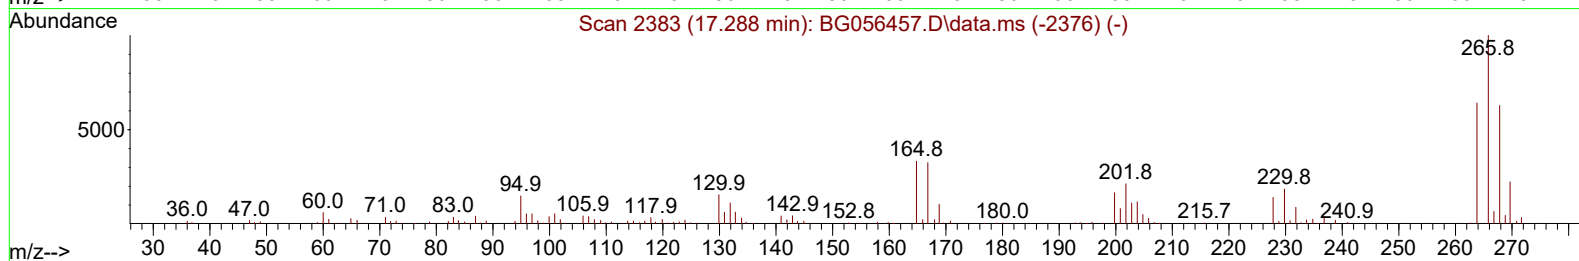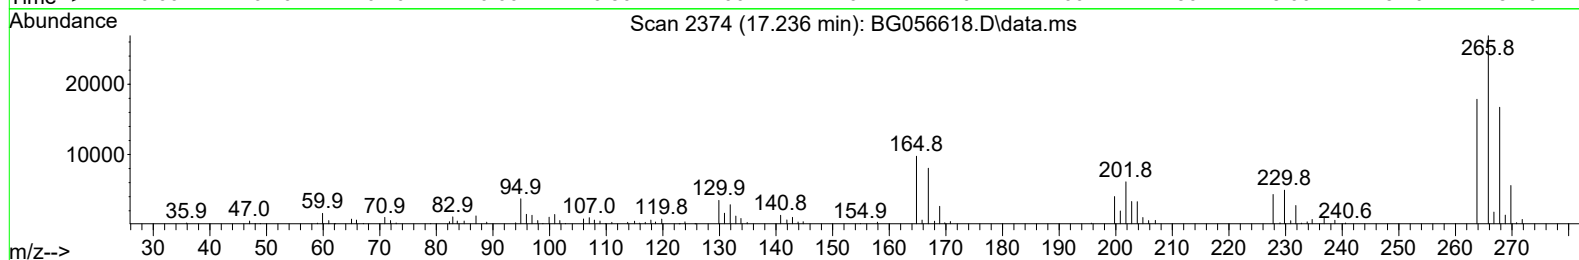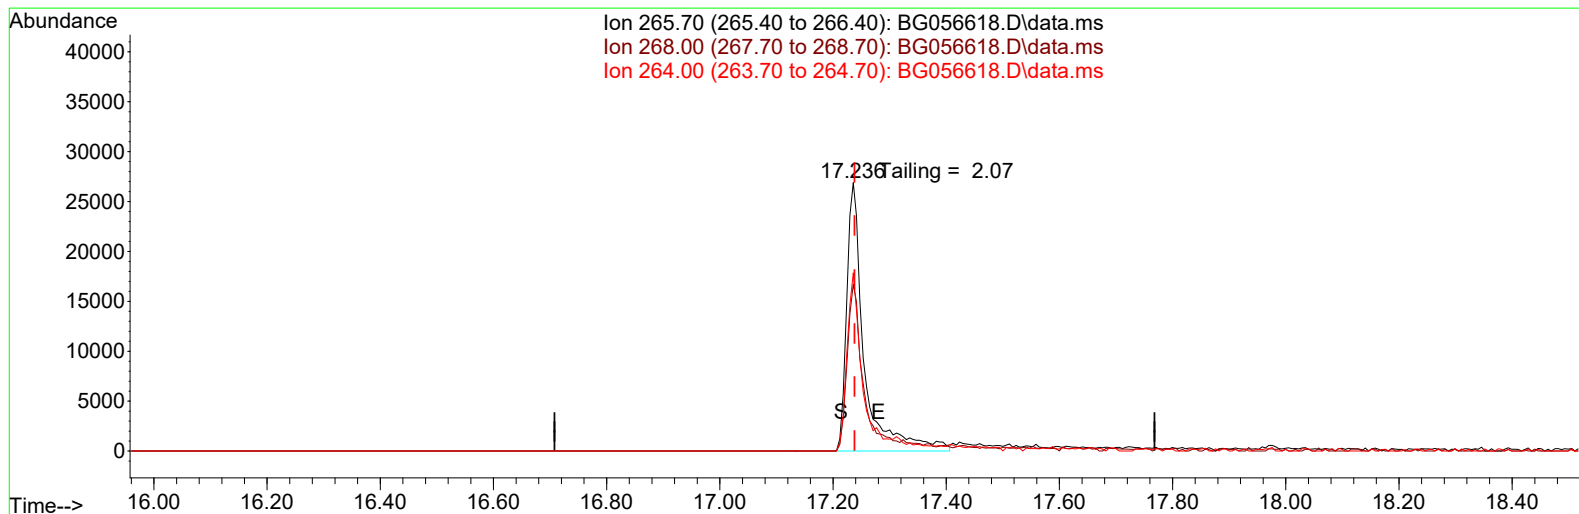

TIC: BG056618.D\data.ms

(70) Pentachlorophenol (C)

17.236min (-0.002) 14508.14 ng




response 56796

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.20
264.00	64.20	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021323\
Data File : BG056618.D
Acq On : 13 Feb 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 14 04:08:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 22:46:08 2023
Response via : Initial Calibration

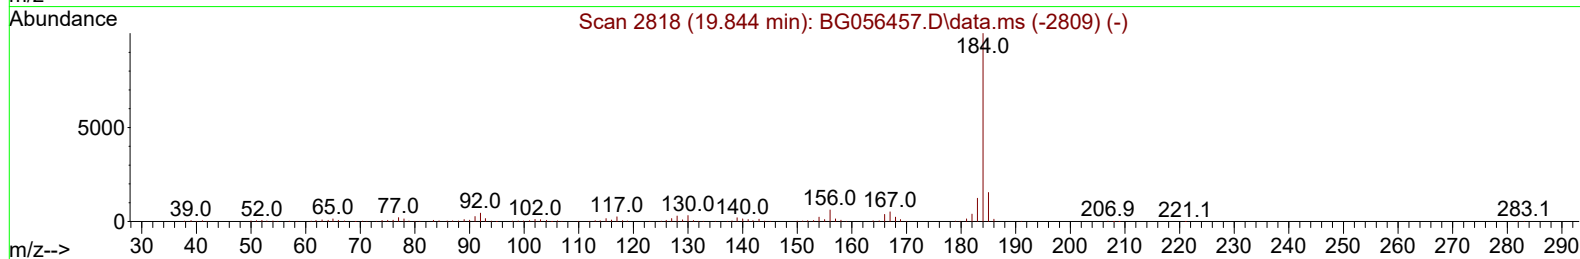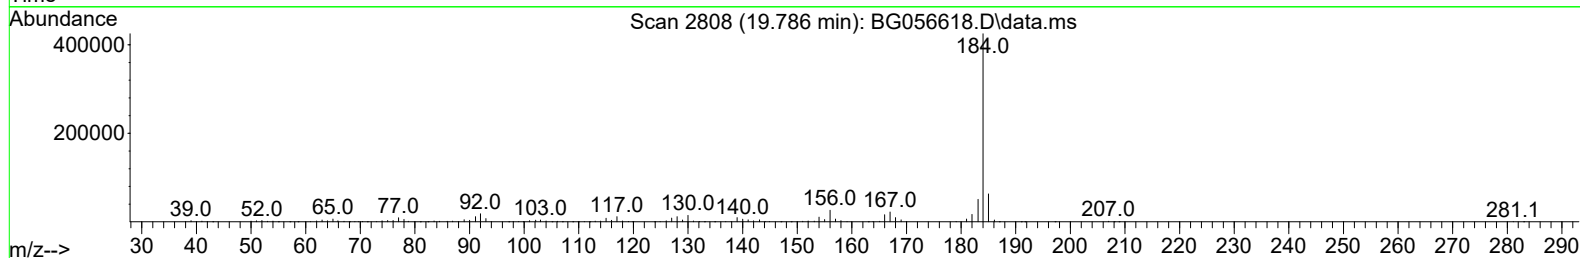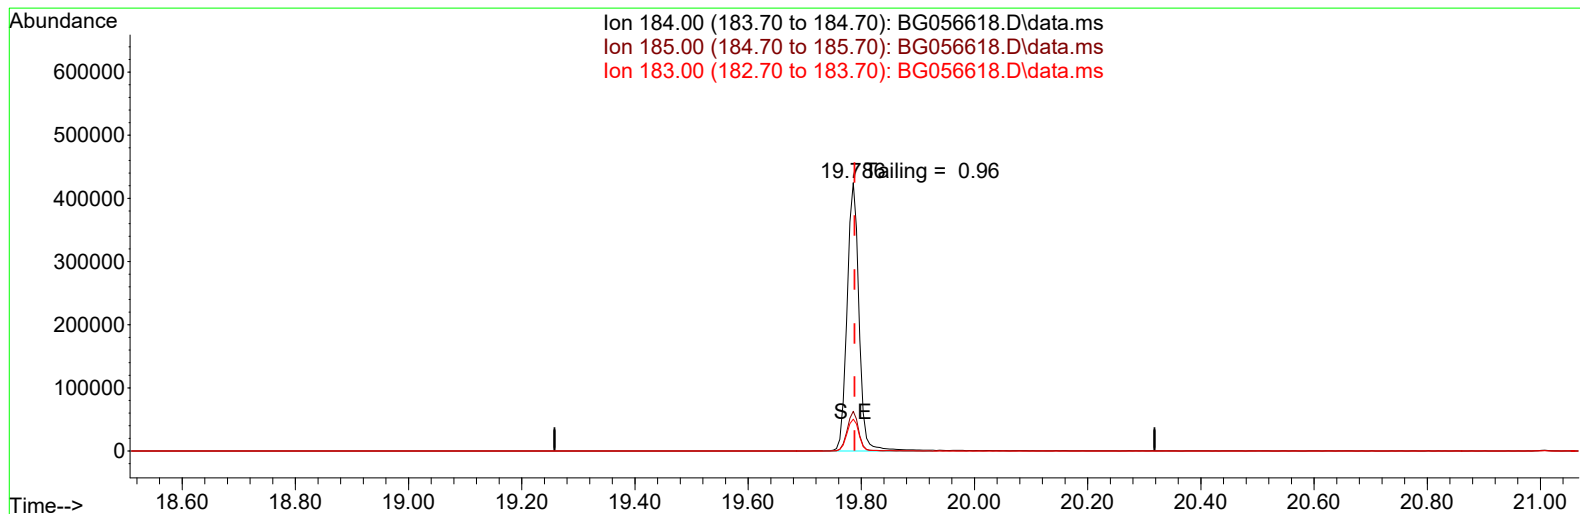

TIC: BG056618.D\data.ms

(77) Benzidine

19.786min (-0.002) 155856.88 ng

response 624216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.82
183.00	12.30	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/13/2023	BNA_G	<u>BG056618.D</u>
Compound Name	Response	Retention Time
DDT	301971	21.008
DDD	11702	20.561
DDE	950	20.062
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12652	314623	4.02

Instrument :
BNA_G
ClientSampleId :
DFTPP