
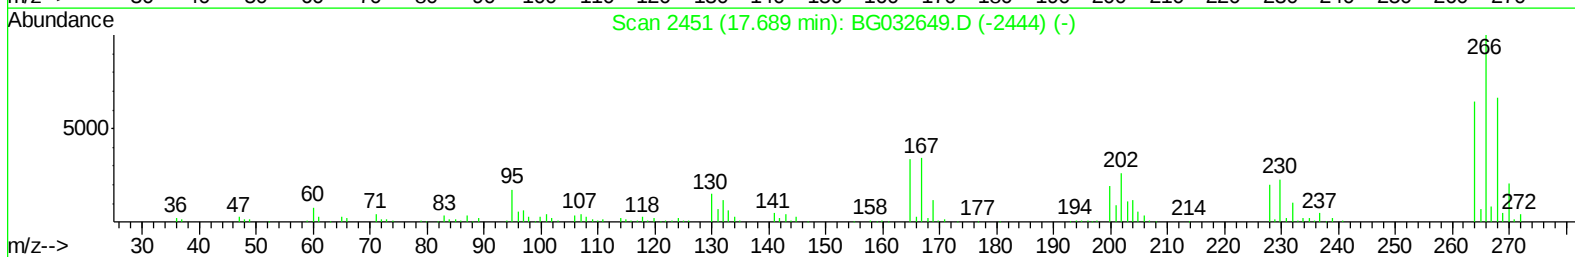
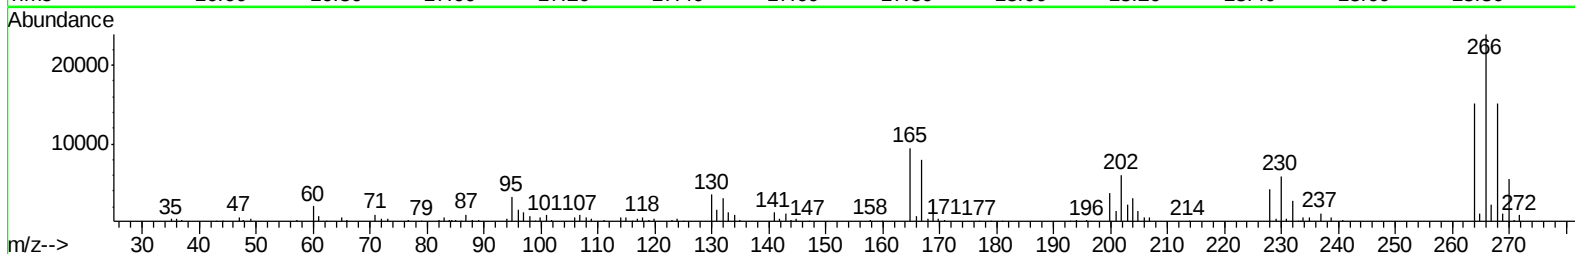


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021418\
Data File : BG032697.D
Acq On : 15 Feb 2018 1:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 07:03:09 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

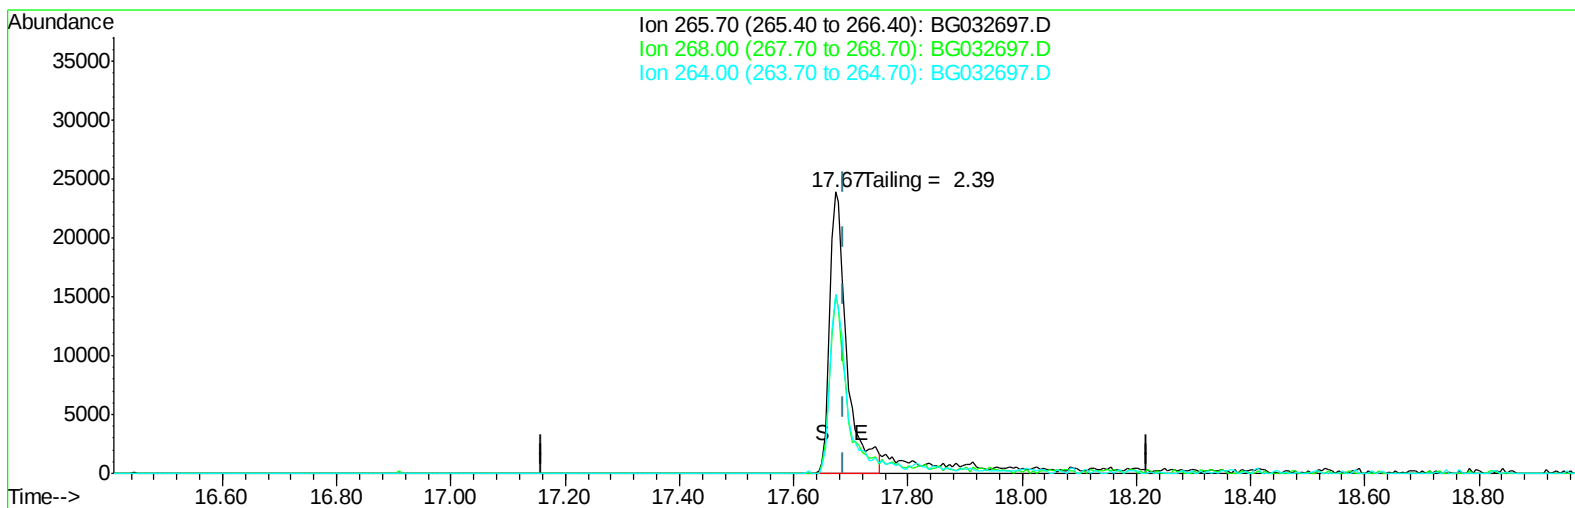

TIC: BG032697.D

(69) Pentachlorophenol (C)




17.673min (-0.016) 12889.94ng

response 48155

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.23
264.00	62.00	63.57
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021418\
Data File : BG032697.D
Acq On : 15 Feb 2018 1:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 07:03:09 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

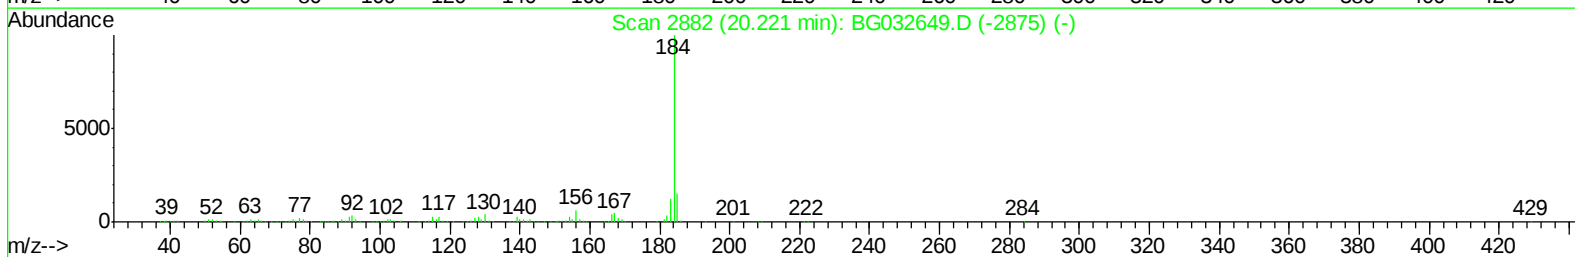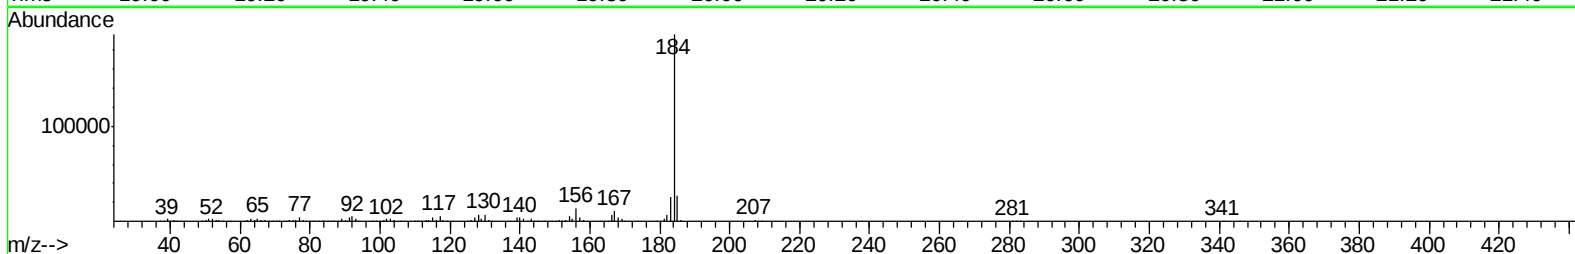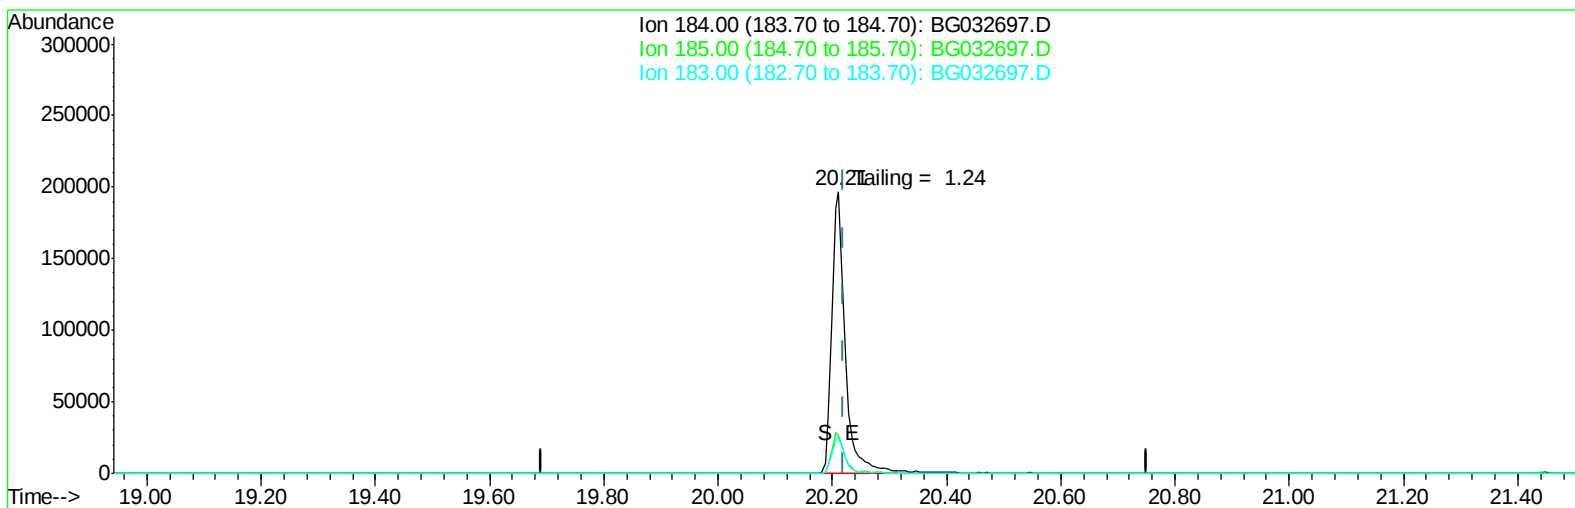

TIC: BG032697.D

(76) Benzidine

20.211min (-0.010) 0.00ng

response 320943

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.64
183.00	13.30	12.84
0.00	0.00	0.00