


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021418\
 Data File : BG032681.D
 Acq On : 14 Feb 2018 13:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 12 18:08:01 2018

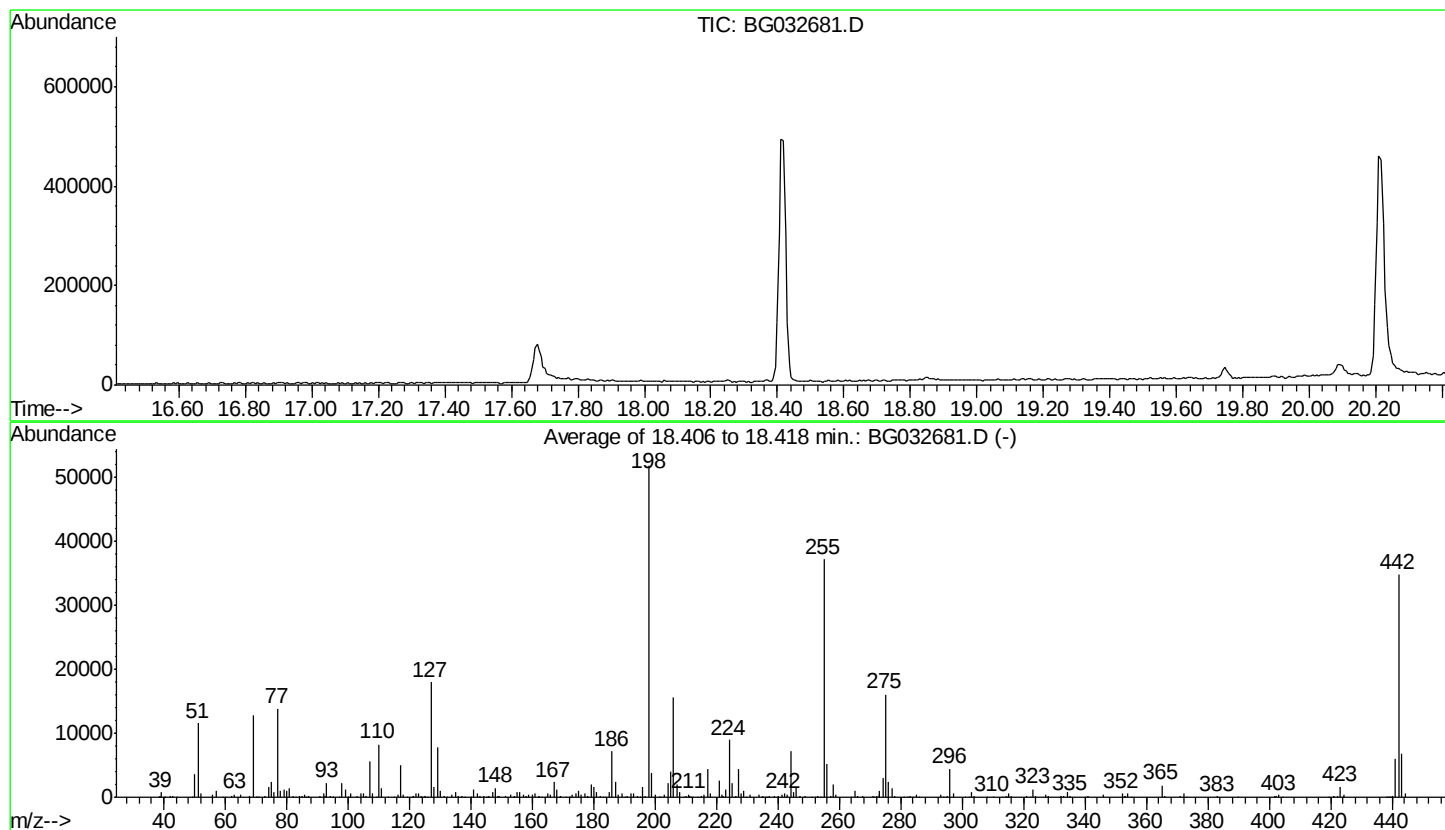

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.3	11549	PASS
68	69	0.00	2	1.2	150	PASS
69	198	0.00	100	24.7	12768	PASS
70	69	0.00	2	0.6	79	PASS
127	198	10	80	34.7	17969	PASS
197	198	0.00	2	0.3	169	PASS
198	198	100	100	100.0	51728	PASS
199	198	5	9	7.3	3789	PASS
275	198	10	60	31.1	16076	PASS
365	198	1	100	3.6	1877	PASS
441	442	0.01	24	17.3	5993	PASS
442	198	50	100	67.0	34674	PASS
443	442	15	24	19.7	6844	PASS