


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021418\
 Data File : BG032697.D
 Acq On : 15 Feb 2018 1:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 12 18:08:01 2018

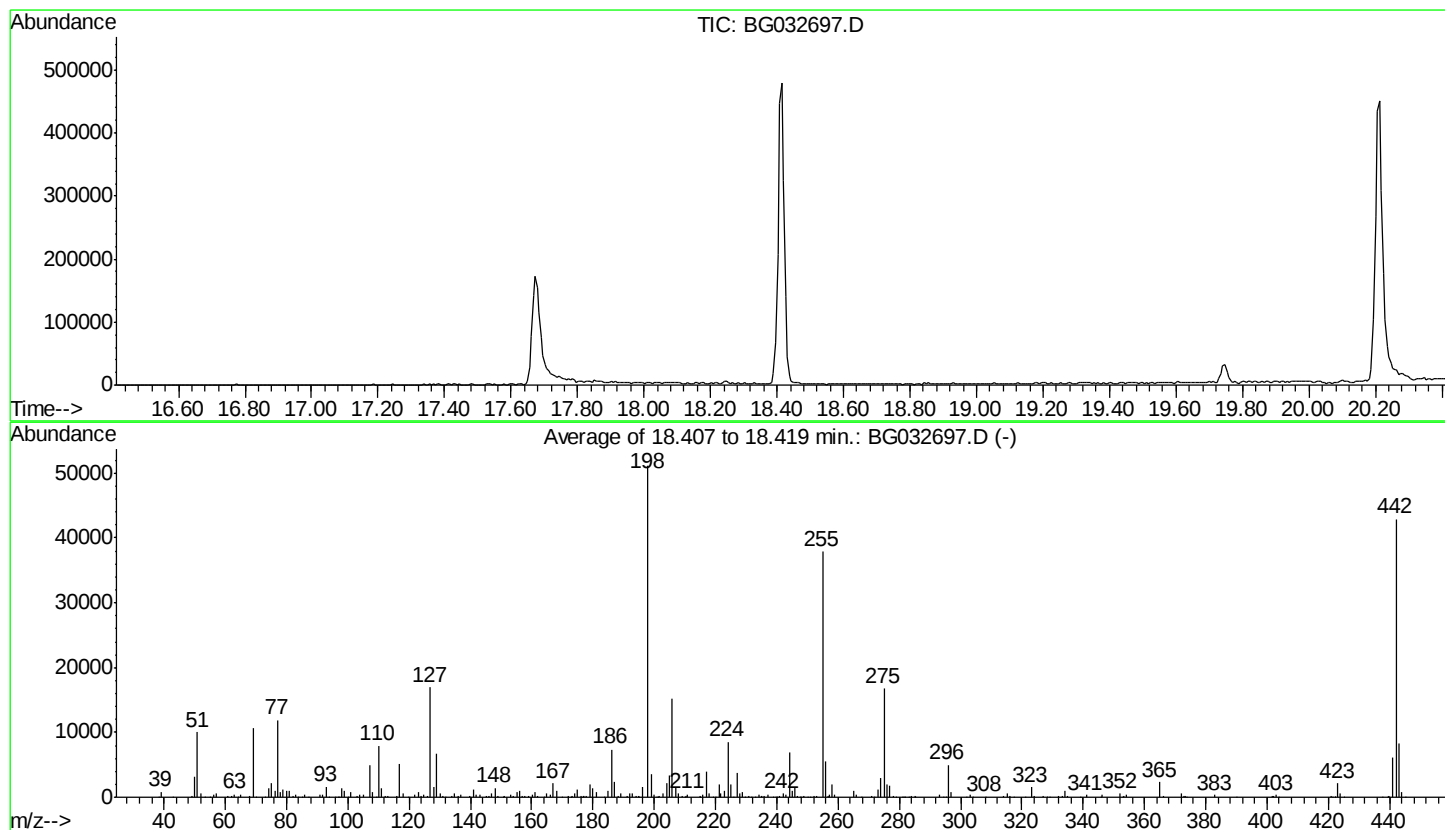

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	10054	PASS
68	69	0.00	2	1.4	146	PASS
69	198	0.00	100	20.7	10599	PASS
70	69	0.00	2	0.6	66	PASS
127	198	10	80	33.0	16895	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51162	PASS
199	198	5	9	6.9	3517	PASS
275	198	10	60	32.6	16697	PASS
365	198	1	100	4.5	2318	PASS
441	442	0.01	24	14.5	6219	PASS
442	198	50	100	83.8	42890	PASS
443	442	15	24	19.2	8233	PASS