

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021419\
 Data File : BG039522.D
 Acq On : 15 Feb 2019 1:13
 Operator : JU/SJ
 Sample : PB117115TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB117115TB

Quant Time: Feb 15 05:38:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	41634	20.00	ng	-0.01
21) Naphthalene-d8	10.99	136	181325	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	135033	20.00	ng	-0.02
64) Phenanthrene-d10	17.53	188	342314	20.00	ng	-0.02
76) Chrysene-d12	21.83	240	358720	20.00	ng	-0.02
87) Perylene-d12	25.21	264	353489	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	340178	139.84	ng	0.00
7) Phenol-d6	7.32	99	510193	142.48	ng	0.00
23) Nitrobenzene-d5	9.35	82	277719	95.68	ng	-0.02
42) 2,4,6-Tribromophenol	16.28	330	171374	117.86	ng	-0.01
45) 2-Fluorobiphenyl	13.42	172	756989	80.42	ng	-0.02
79) Terphenyl-d14	20.13	244	1291509	76.21	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021419\
Data File : BG039522.D
Acq On : 15 Feb 2019 1:13
Operator : JU/SJ
Sample : PB117115TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117115TB

Quant Time: Feb 15 05:38:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

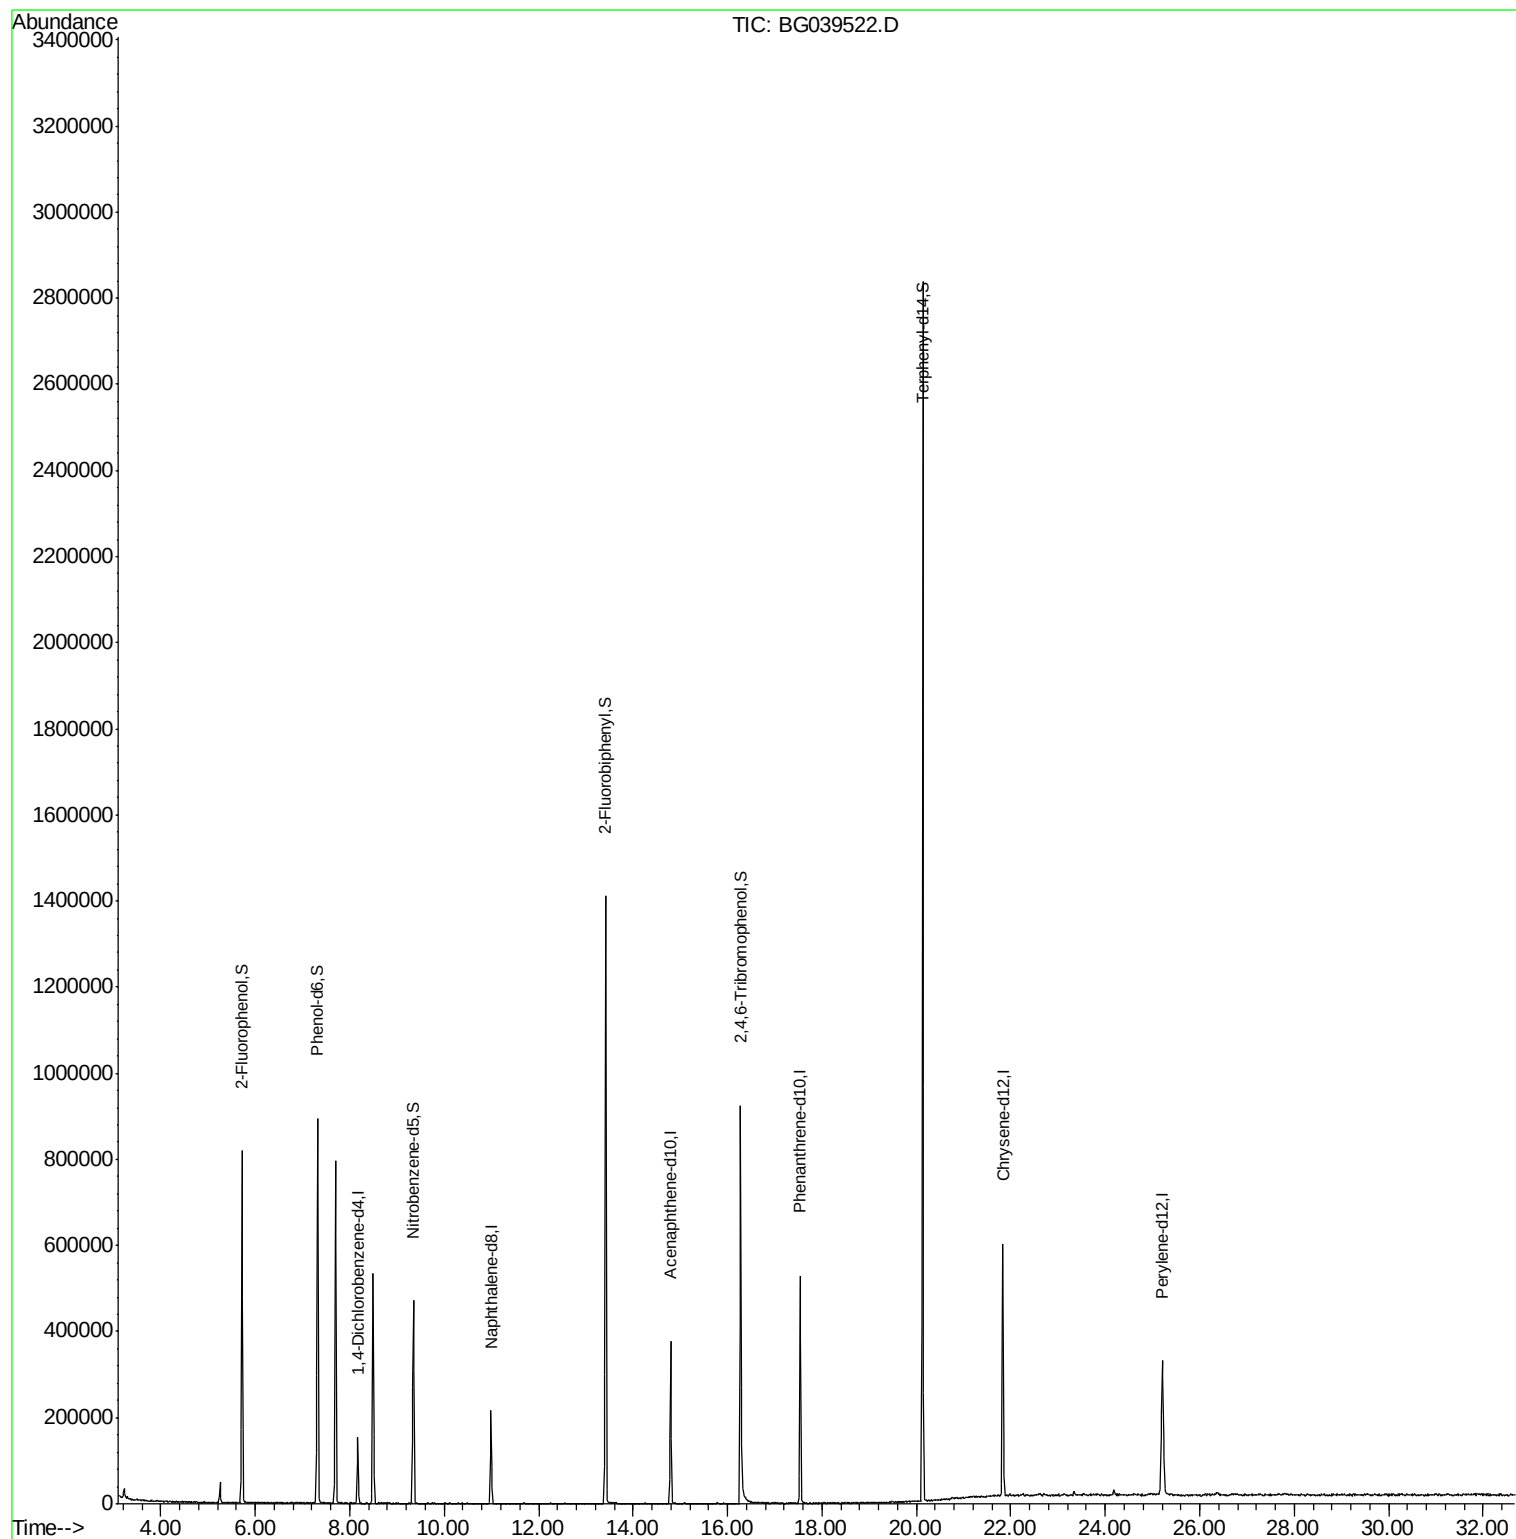

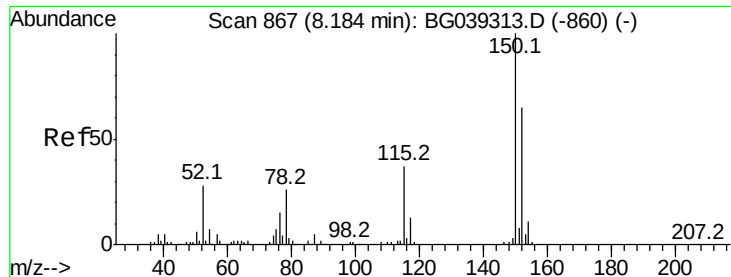


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 865
Delta R.T. -0.01 min
Lab File: BG039522.D
Acq: 15 Feb 2019 1:13

Instrument :
BNA_G
ClientSampleId :
PB117115TB

Tot Ion:152 Resp: 41634
Ion Ratio Lower Upper
152 100
150 153.4 123.7 185.5
115 61.4 45.9 68.9

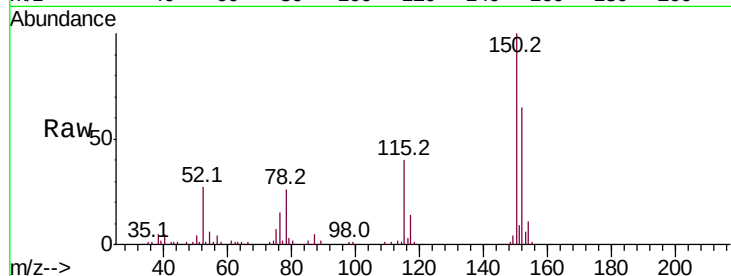


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

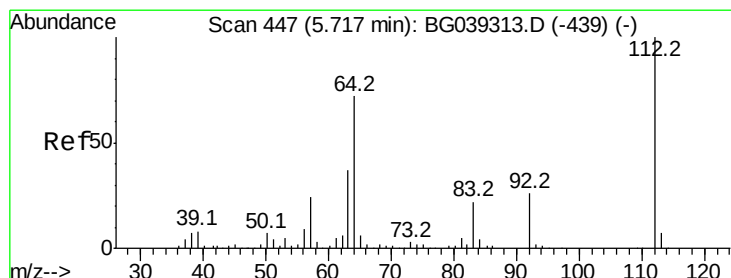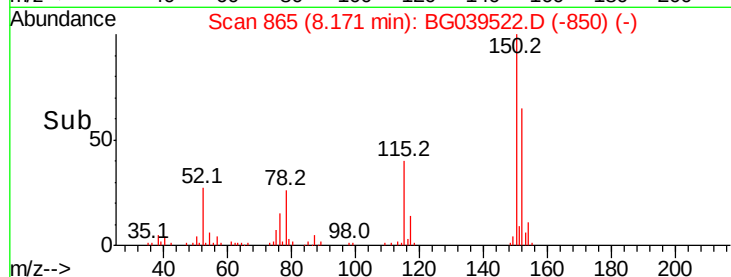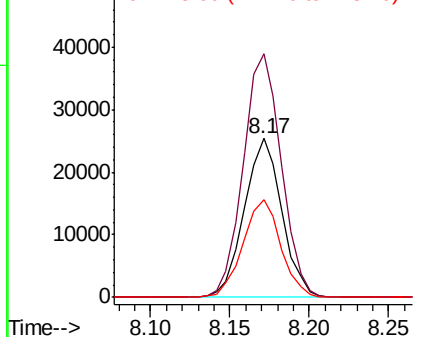



#5


2-Fluorophenol
Concen: 139.842 ng
RT: 5.72 min Scan# 447
Delta R.T. -0.00 min
Lab File: BG039522.D
Acq: 15 Feb 2019 1:13

Tgt Ion:112 Resp: 340178
Ion Ratio Lower Upper
112 100
64 71.1 57.8 86.8
63 37.6 29.8 44.6

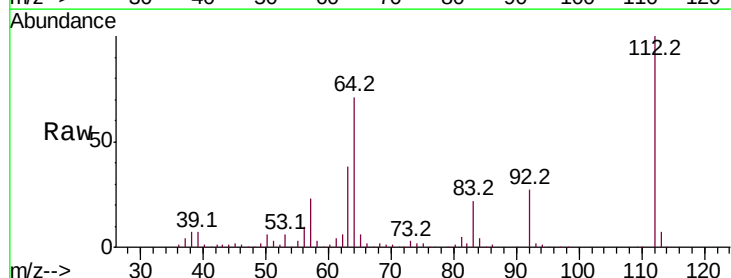

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

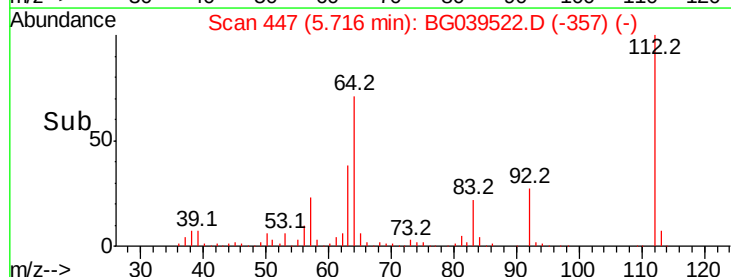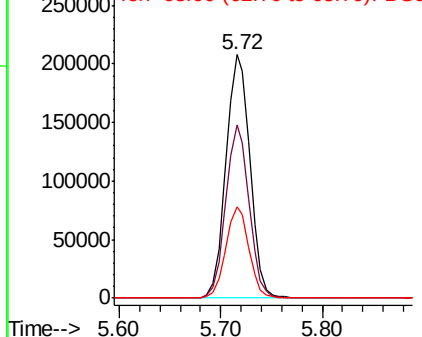

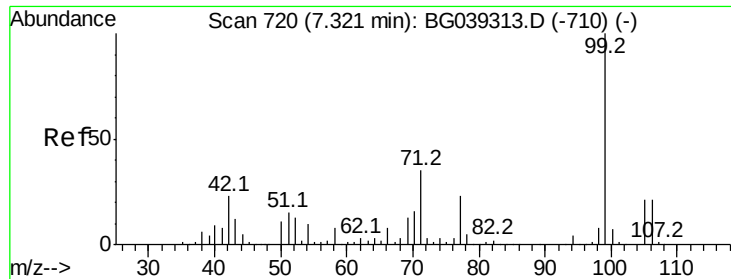

#7

Phenol-d6

Concen: 142.484 ng

RT: 7.32 min Scan# 720

Delta R.T. -0.00 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13

Instrument :

BNA_G

ClientSampleId :

PB117115TB


Tot Ion: 99 Resp: 510193

Ion Ratio Lower Upper




99 100

42 21.2 18.2 27.2

71 36.6 28.0 42.0

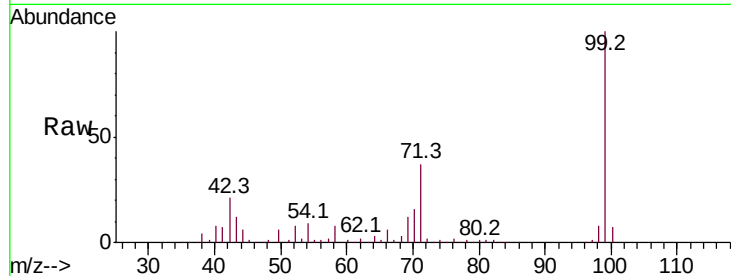

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

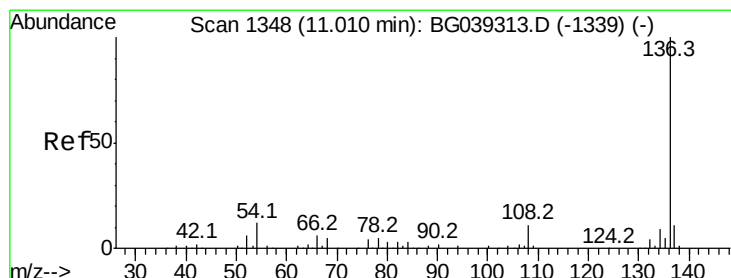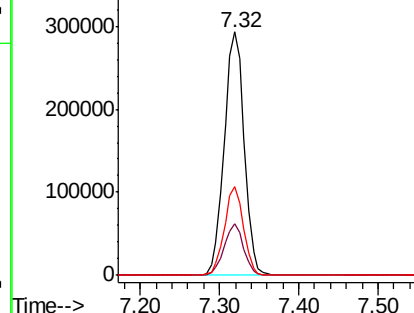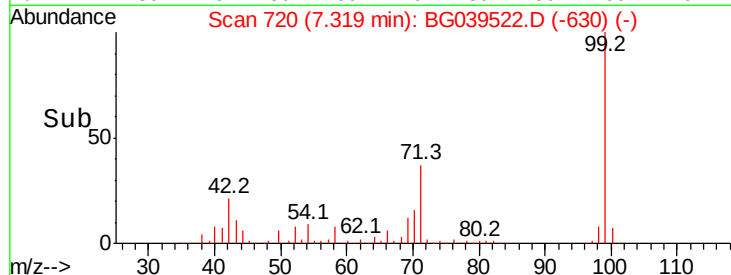

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1345

Delta R.T. -0.02 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13

Tgt Ion: 136 Resp: 181325


Ion Ratio Lower Upper

136 100



137 11.1 9.1 13.7


54 11.1 9.4 14.2

68 6.1 4.2 6.4

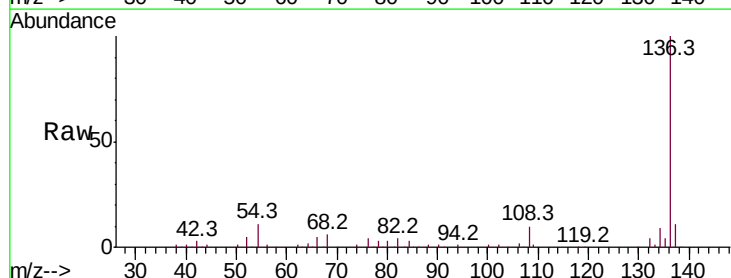

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



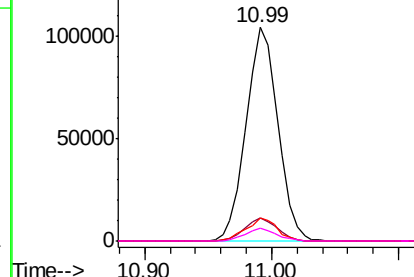
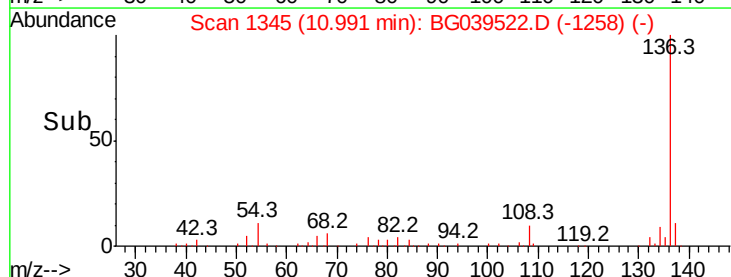


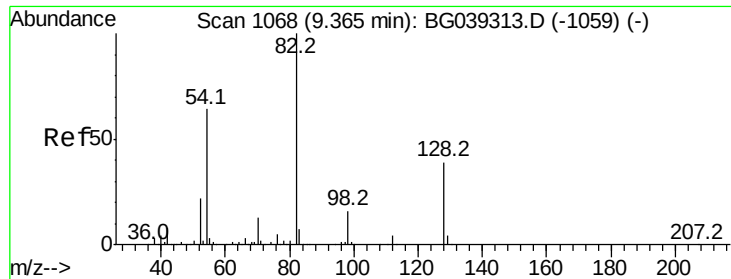

#23
 Nitrobenzene-d5
 Concen: 95.682 ng
 RT: 9.35 min Scan# 1065
 Delta R.T. -0.02 min
 Lab File: BG039522.D
 Acq: 15 Feb 2019 1:13




Instrument :
 BNA_G
 ClientSampleId :
 PB117115TB


Tot Ion: 82 Resp: 277719
 Ion Ratio Lower Upper
 82 100
 128 44.5 31.3 46.9
 54 59.8 50.9 76.3

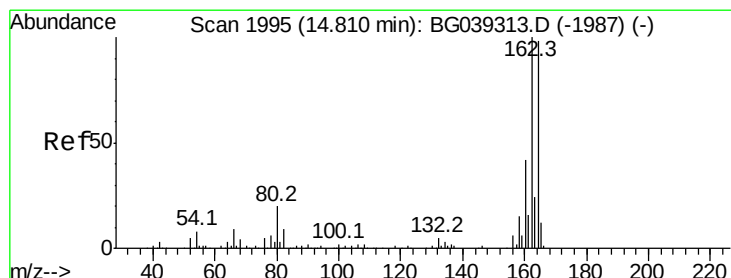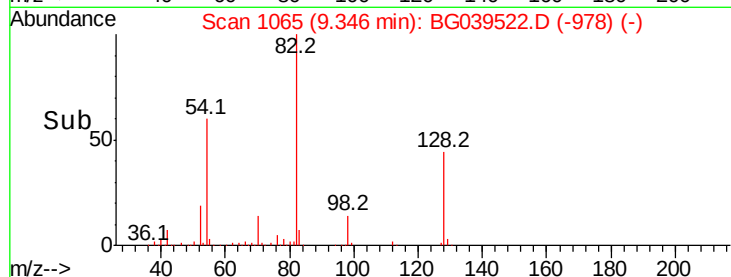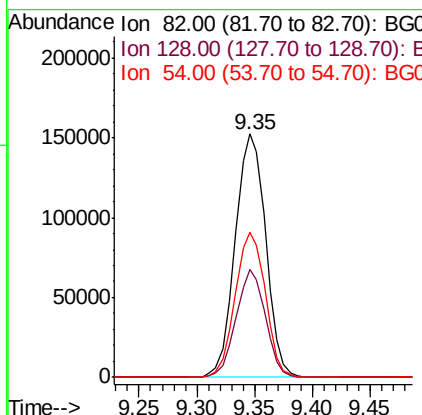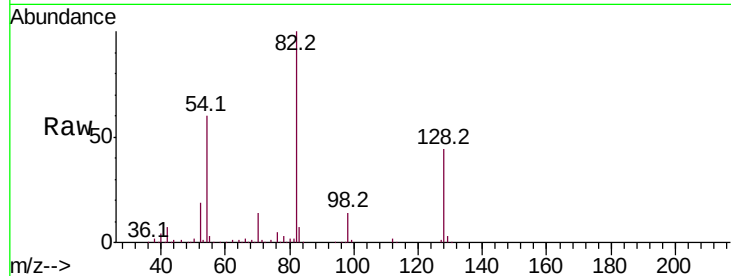

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1992
 Delta R.T. -0.02 min
 Lab File: BG039522.D
 Acq: 15 Feb 2019 1:13

Tgt Ion: 164 Resp: 135033
 Ion Ratio Lower Upper
 164 100
 162 102.3 81.6 122.4
 160 43.3 34.2 51.2

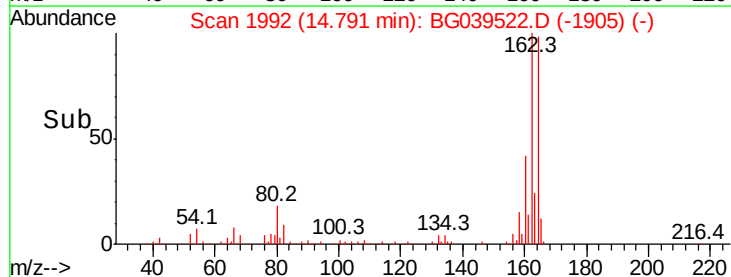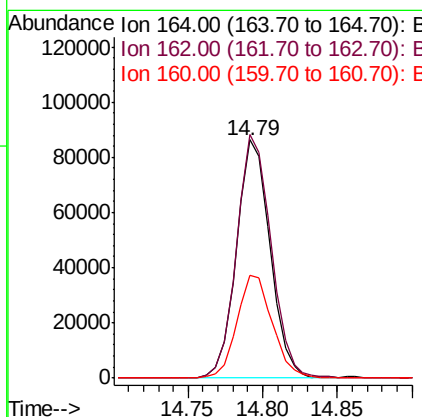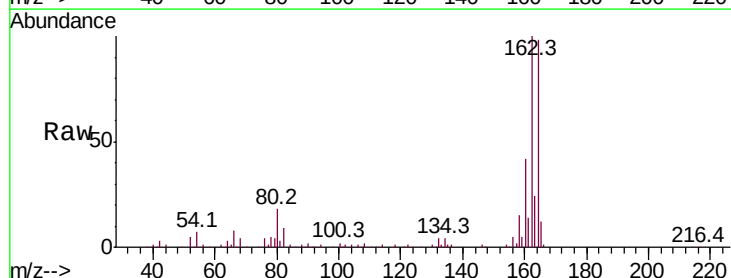

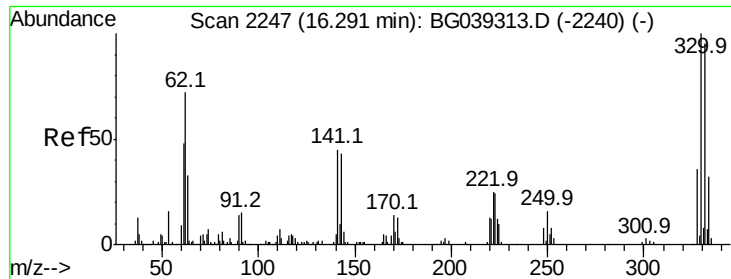

#42

2,4,6-Tribromophenol

Concen: 117.858 ng

RT: 16.28 min Scan# 2245

Delta R.T. -0.01 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13

Instrument :

BNA_G

ClientSampleId :

PB117115TB


Tot Ion:330 Resp: 171374

Ion Ratio Lower Upper

330 100

332 99.0 75.7 113.5




141 41.6 35.6 53.4

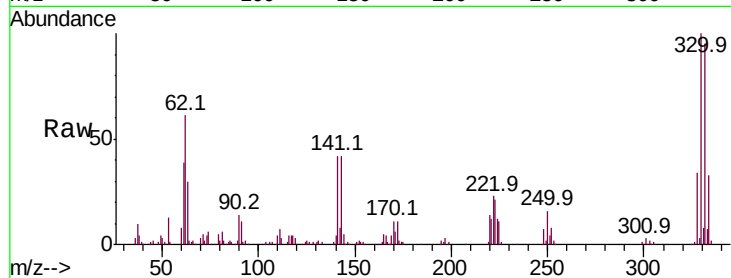

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

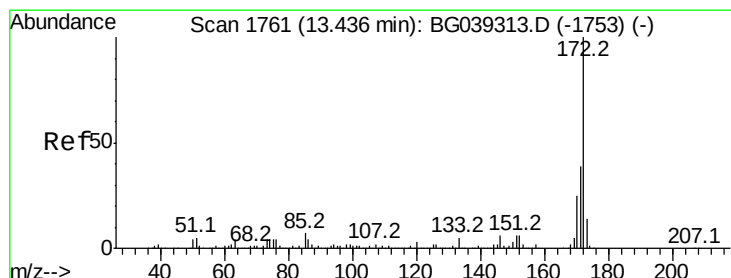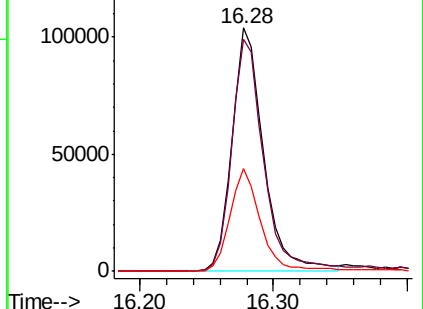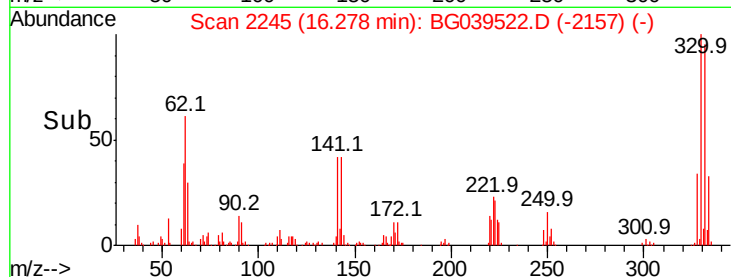

#45

2-Fluorobiphenyl

Concen: 80.420 ng

RT: 13.42 min Scan# 1758

Delta R.T. -0.02 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13


Tgt Ion:172 Resp: 756989

Ion Ratio Lower Upper

172 100

171 37.3 30.8 46.2



170 24.2 20.2 30.4

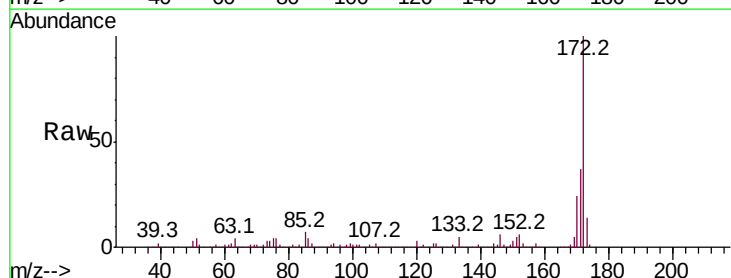


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

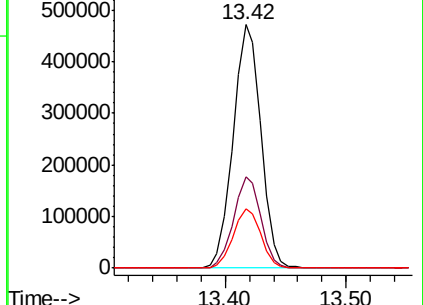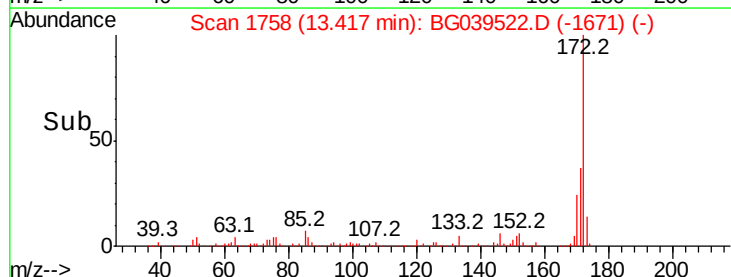

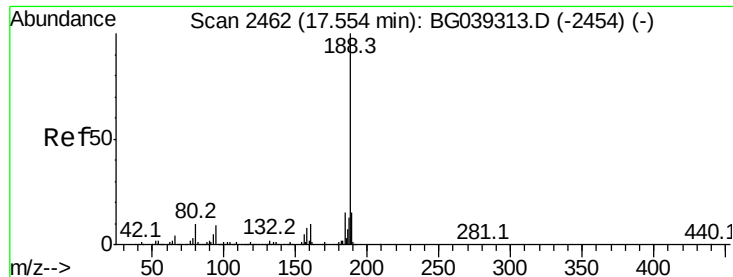

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.53 min Scan# 2459

Delta R.T. -0.02 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13

Instrument :

BNA_G

ClientSampleId :

PB117115TB


Tot Ion:188 Resp: 342314

Ion Ratio Lower Upper

188 100

94 8.4 6.9 10.3




80 8.9 8.1 12.1

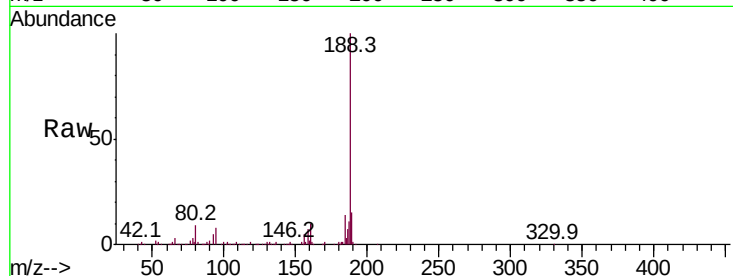

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

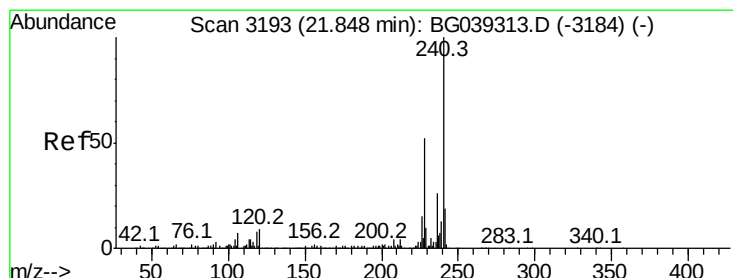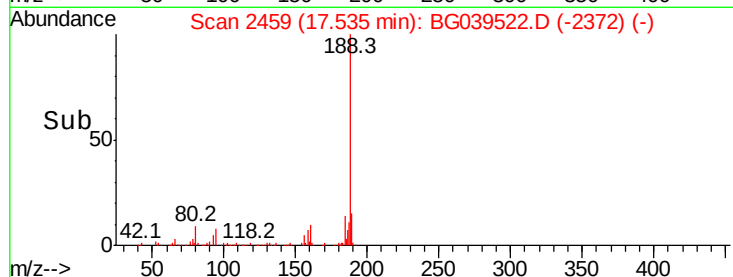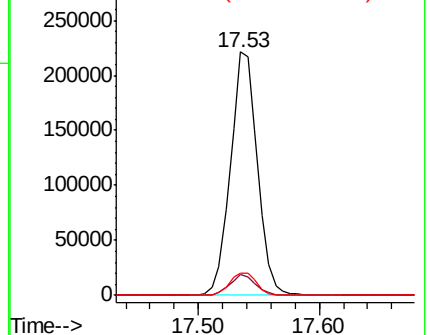

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.83 min Scan# 3190

Delta R.T. -0.02 min

Lab File: BG039522.D

Acq: 15 Feb 2019 1:13


Tgt Ion:240 Resp: 358720

Ion Ratio Lower Upper

240 100

120 8.9 7.0 10.6



236 26.3 21.0 31.4

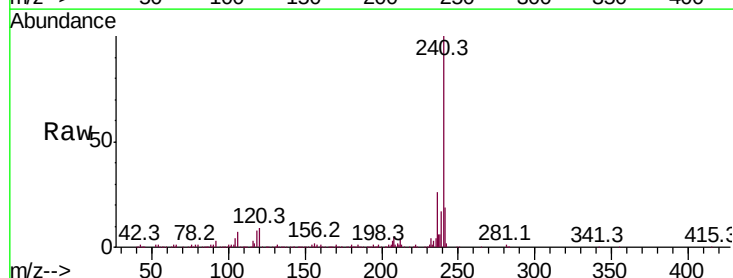


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



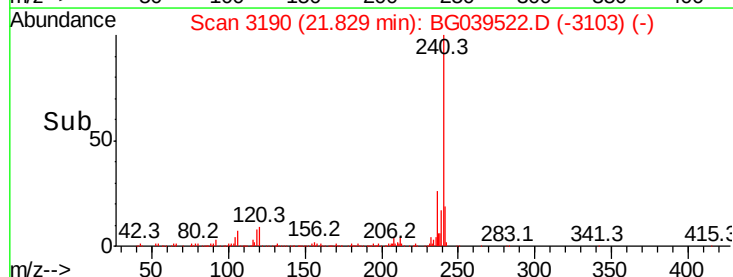
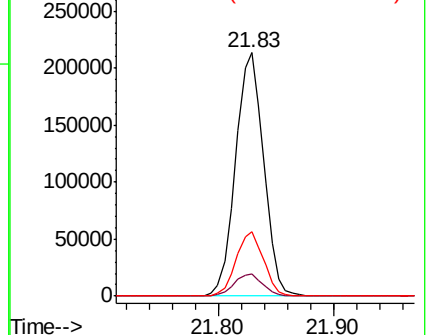


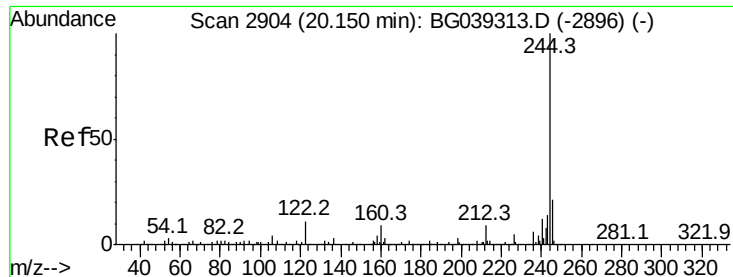

#79
 Terphenyl-d14
 Concen: 76.208 ng
 RT: 20.13 min Scan# 2901
 Delta R.T. -0.02 min
 Lab File: BG039522.D
 Acq: 15 Feb 2019 1:13

Instrument :
 BNA_G
 ClientSampleId :
 PB117115TB

Tot Ion:244 Resp: 1291509
 Ion Ratio Lower Upper
 244 100
 212 8.8 7.3 10.9
 122 10.0 8.4 12.6

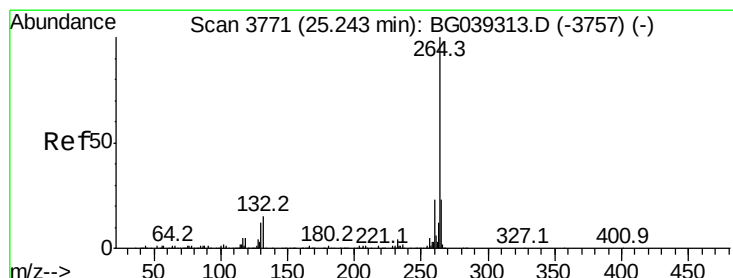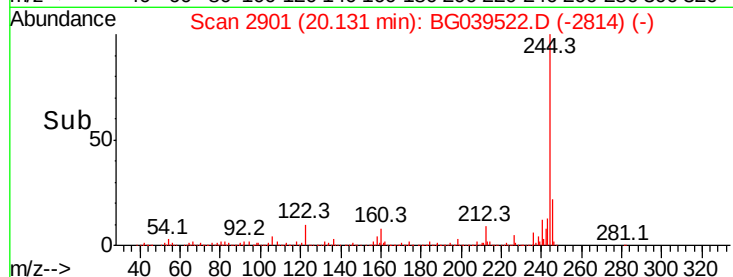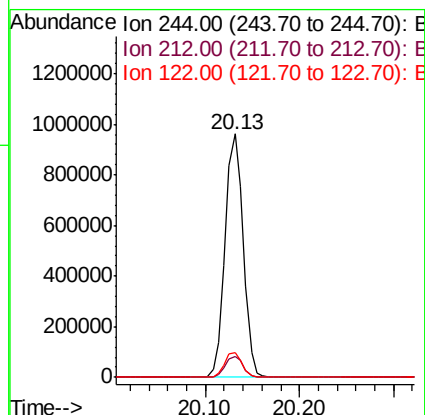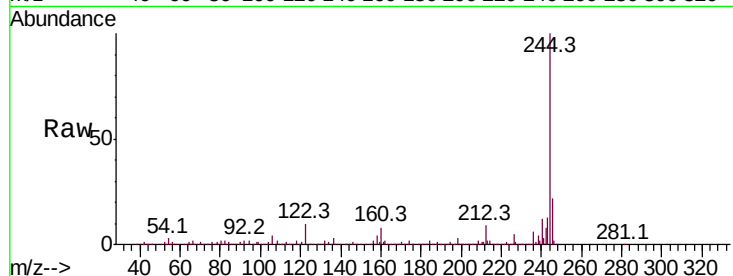

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.21 min Scan# 3765
 Delta R.T. -0.04 min
 Lab File: BG039522.D
 Acq: 15 Feb 2019 1:13

Tgt Ion:264 Resp: 353489
 Ion Ratio Lower Upper
 264 100
 260 25.6 18.2 27.4
 265 20.5 18.5 27.7

