


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021419\
 Data File : BG039509.D
 Acq On : 14 Feb 2019 15:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

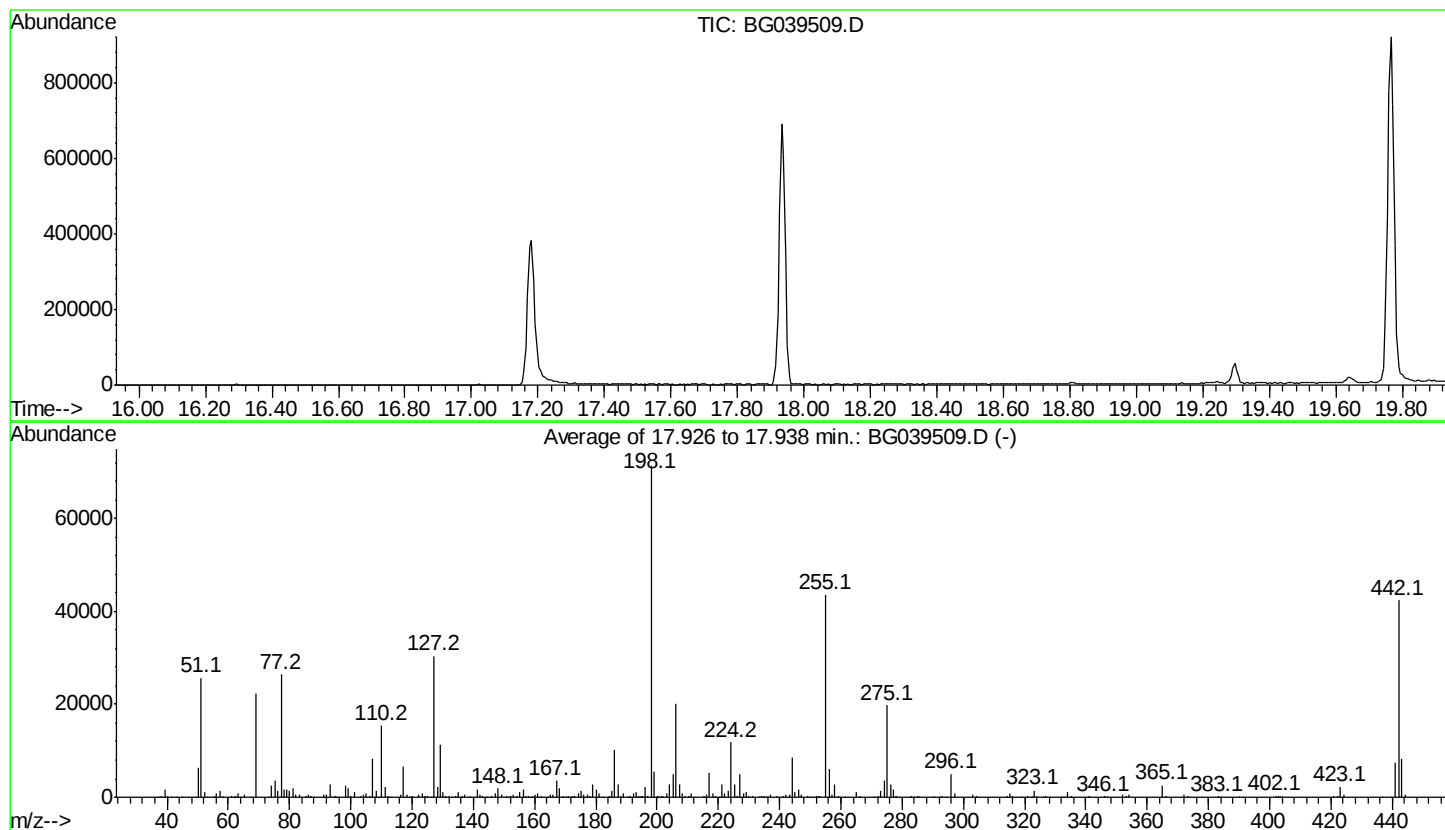

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	25739	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.2	22267	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	30373	PASS
197	198	0.00	2	0.4	317	PASS
198	198	100	100	100.0	71360	PASS
199	198	5	9	7.6	5411	PASS
275	198	10	60	27.7	19738	PASS
365	198	1	100	3.5	2526	PASS
441	198	0.01	100	10.3	7354	PASS
442	198	50	100	59.3	42314	PASS
443	442	15	24	19.5	8242	PASS