
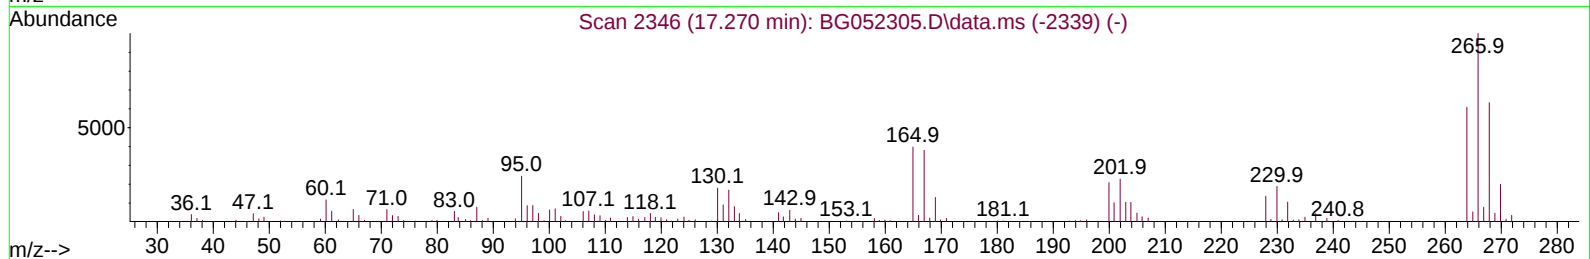
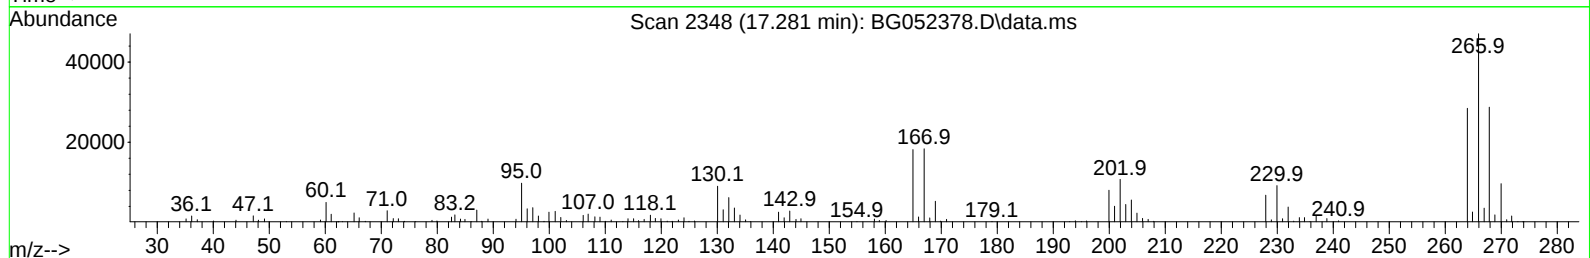


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052378.D
Acq On : 14 Feb 2022 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 14:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

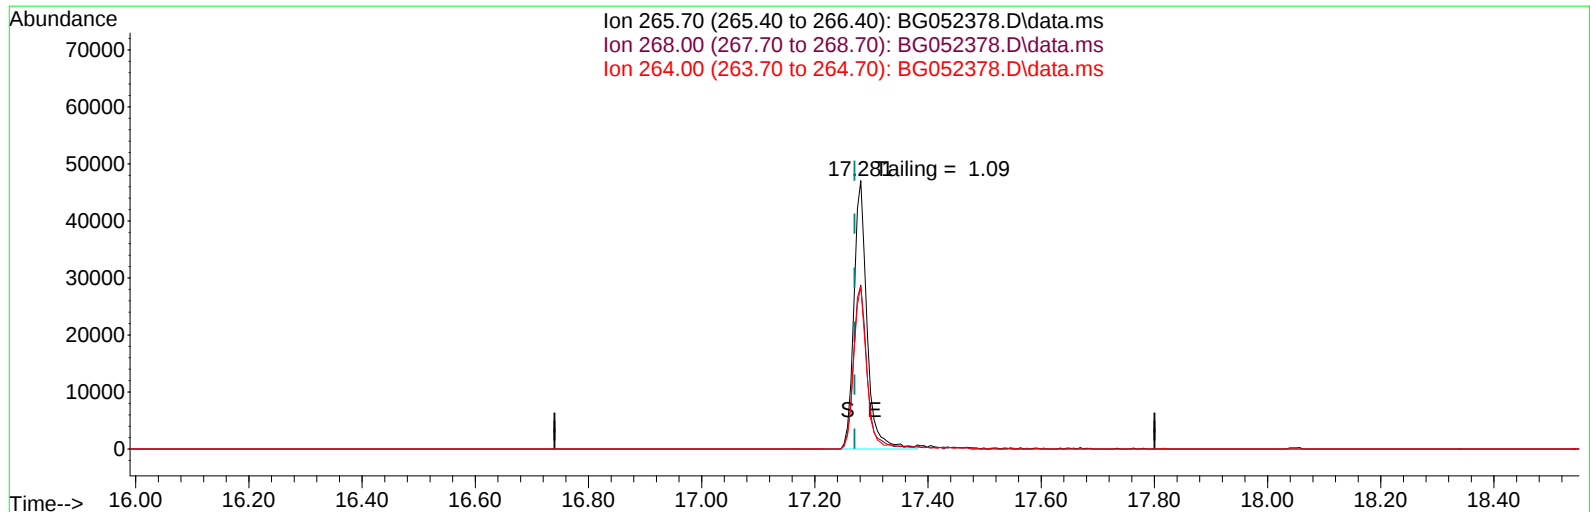

TIC: BG052378.D\data.ms

(70) Pentachlorophenol (C)




17.281min (+ 0.011) 25797.17 ng

response 75575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.06
264.00	65.20	60.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052378.D
Acq On : 14 Feb 2022 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 14:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

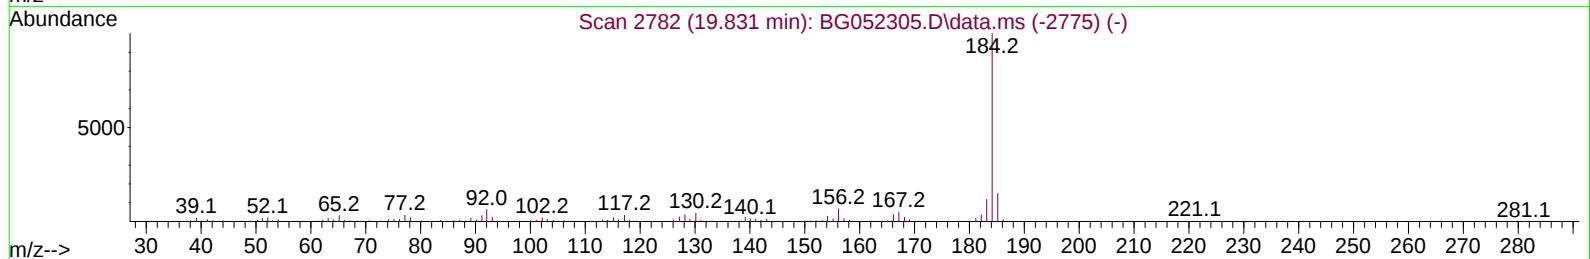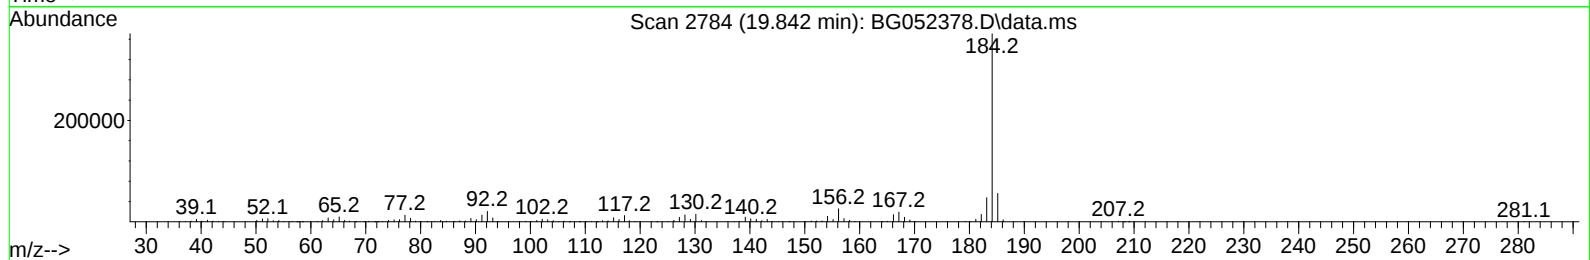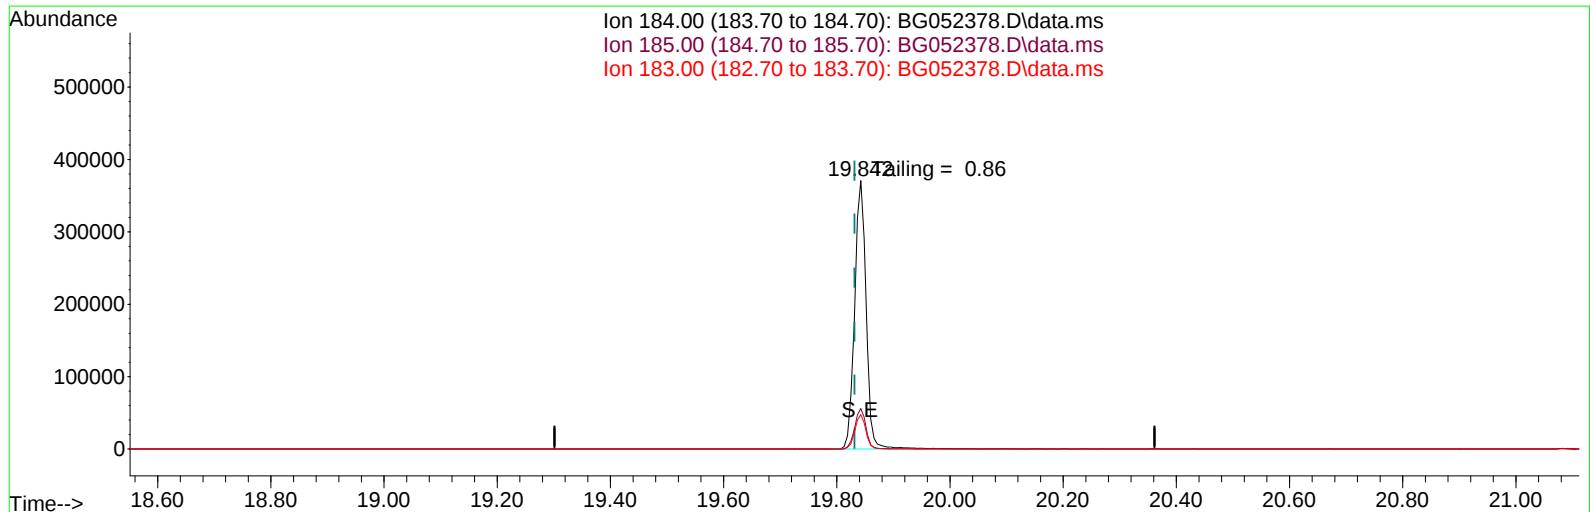

TIC: BG052378.D\data.ms

(77) Benzidine

19.842min (+ 0.011) 0.00 ng

response 523820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.11
183.00	12.20	12.81
0.00	0.00	0.00