

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
 Data File : BG052381.D
 Acq On : 14 Feb 2022 13:27
 Operator : CG/JU
 Sample : PB142473BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB142473BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.755	378	386	398	rBV	489065	776324	27.99%	7.970%
2	7.371	654	661	676	rVB	486257	831029	29.96%	8.531%
3	8.223	796	806	814	rBV	87811	146283	5.27%	1.502%
4	9.398	998	1006	1016	rBV	310386	551326	19.88%	5.660%
5	11.060	1282	1289	1298	rBV	118512	213344	7.69%	2.190%
6	13.492	1696	1703	1716	rBV	859538	1338193	48.25%	13.738%
7	14.867	1929	1937	1950	rBV	207022	327467	11.81%	3.362%
8	16.359	2184	2191	2207	rBV	643206	1050553	37.88%	10.785%
9	17.622	2399	2406	2416	rBV	293215	453024	16.33%	4.651%
10	20.212	2841	2847	2853	rBV	2137756	2773631	100.00%	28.474%
11	21.934	3133	3140	3149	rVB2	326245	557448	20.10%	5.723%
12	24.389	3552	3558	3568	rVB4	15062	34130	1.23%	0.350%
13	25.405	3718	3731	3743	rBV2	188190	584262	21.06%	5.998%
14	26.662	3937	3945	3957	rVB7	17544	55311	1.99%	0.568%
15	28.149	4192	4198	4211	rVB7	15783	48750	1.76%	0.500%




Sum of corrected areas: 9741075

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052381.D
Acq On : 14 Feb 2022 13:27
Operator : CG/JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

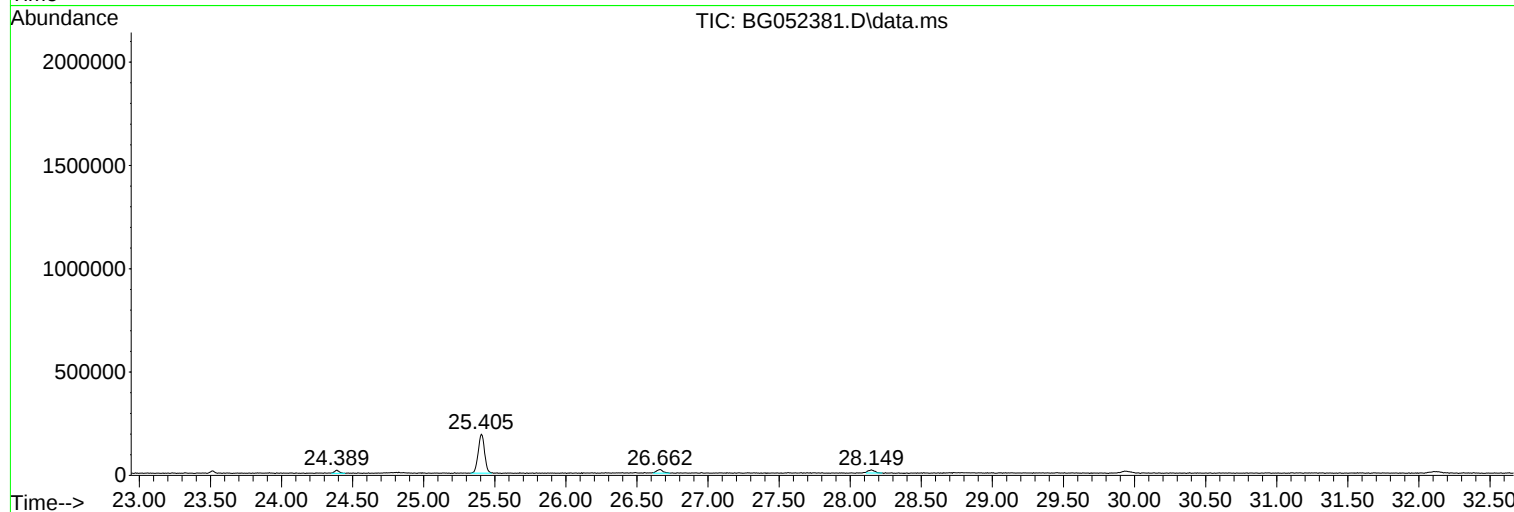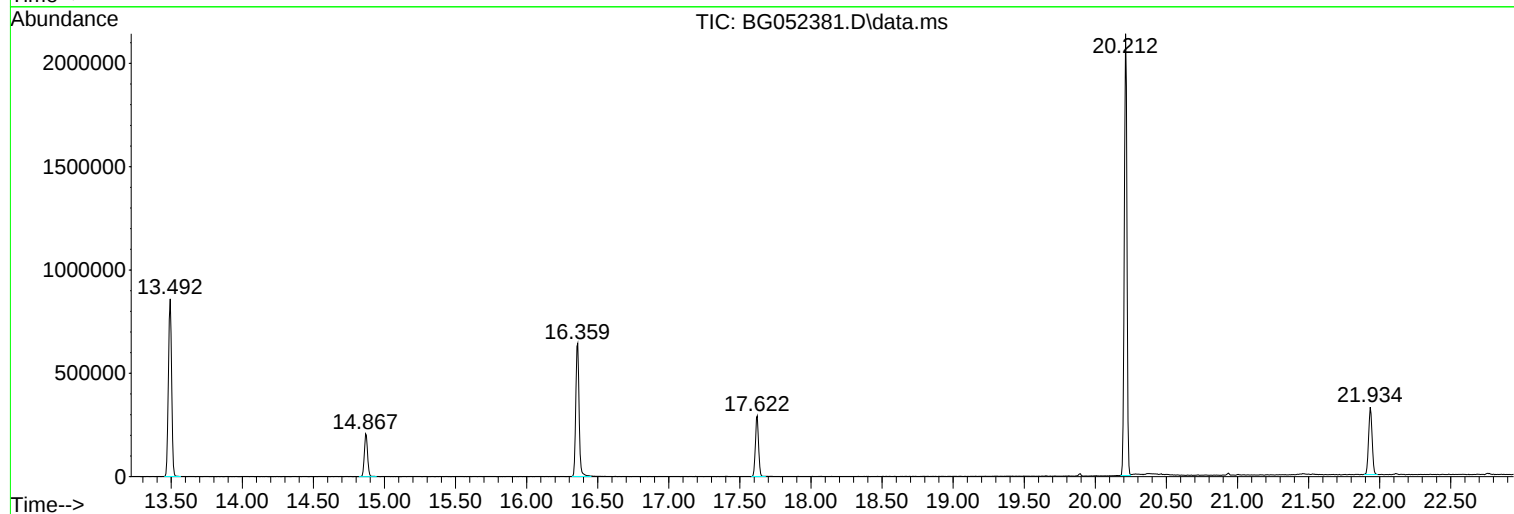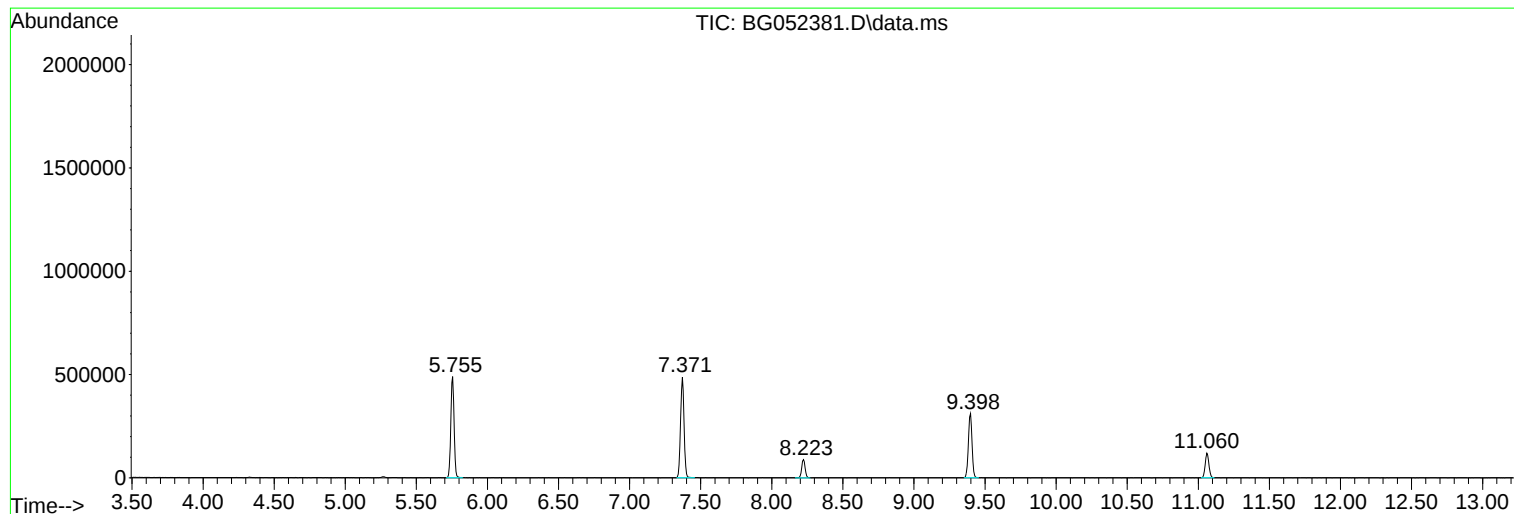

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052381.D
Acq On : 14 Feb 2022 13:27
Operator : CG/JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052381.D
Acq On : 14 Feb 2022 13:27
Operator : CG/JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------