


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
 Data File : BG052378.D
 Acq On : 14 Feb 2022 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

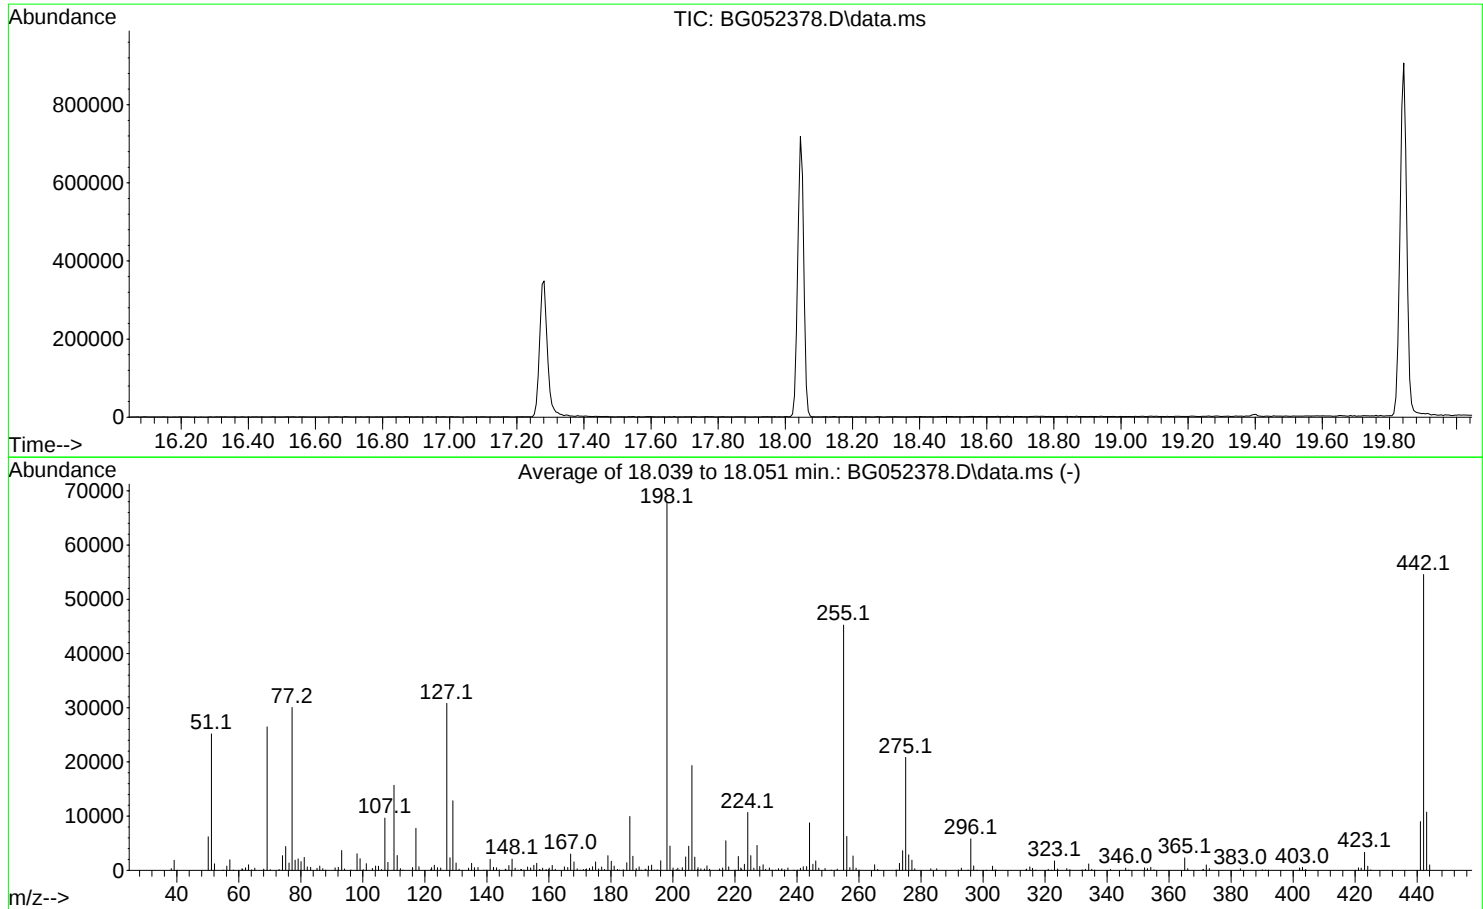

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	25184	PASS
68	69	0.00	2	0.9	235	PASS
69	198	0.00	100	39.0	26469	PASS
70	69	0.00	2	0.4	117	PASS
127	198	10	80	45.4	30808	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67853	PASS
199	198	5	9	6.6	4497	PASS
275	198	10	60	30.7	20832	PASS
365	198	1	100	3.4	2300	PASS
441	198	0.01	100	13.3	8998	PASS
442	442	50	100	100.0	54565	PASS
443	442	15	24	19.7	10750	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/14/2022	BNA_G	<u>BG052378.D</u>
Compound Name	Response	Retention Time
DDT	267477	21.08
DDD	2551	20.63
DDE	364	20.13
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2915	270392	1.08

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052378.D
Acq On : 14 Feb 2022 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 14 14:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

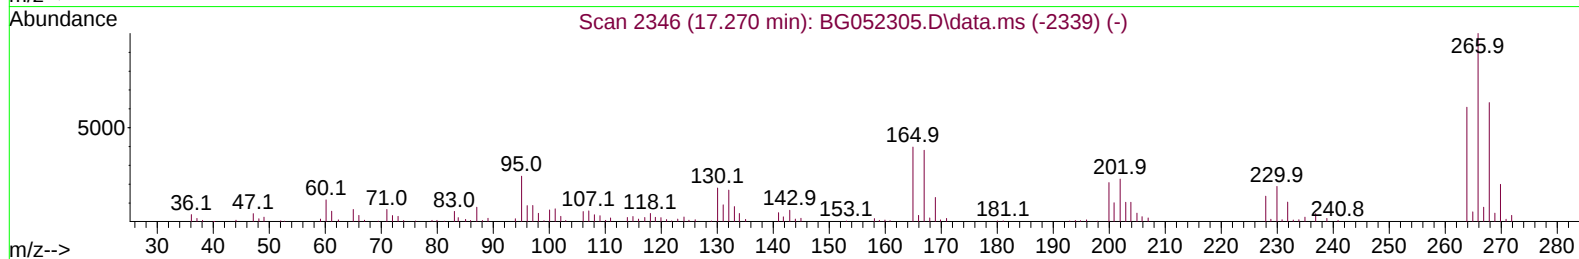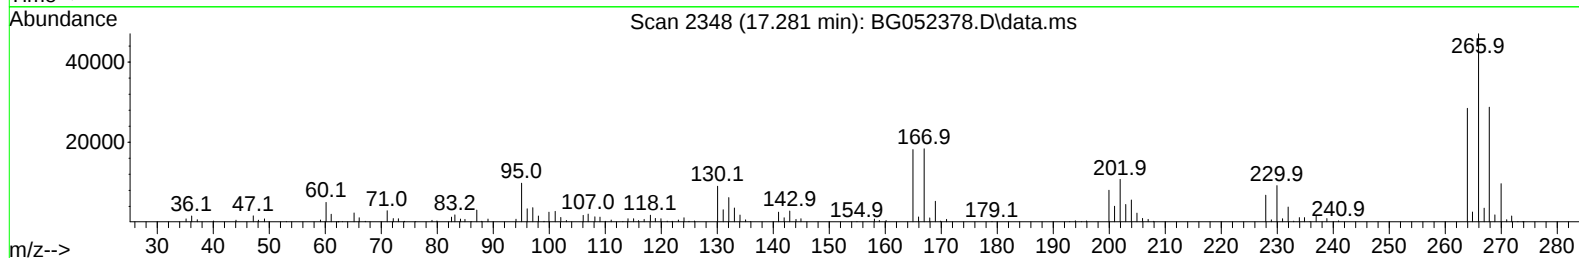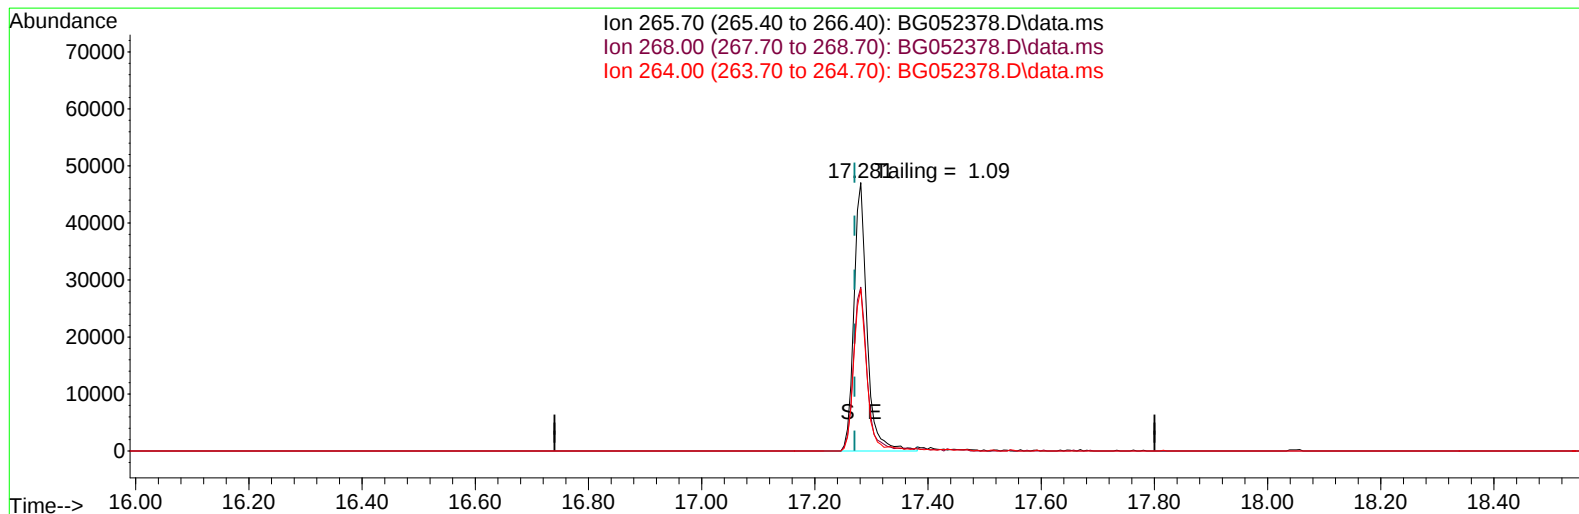

TIC: BG052378.D\data.ms

(70) Pentachlorophenol (C)

17.281min (+ 0.011) 25797.17 ng




response 75575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.06
264.00	65.20	60.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021422\
Data File : BG052378.D
Acq On : 14 Feb 2022 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 14 14:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

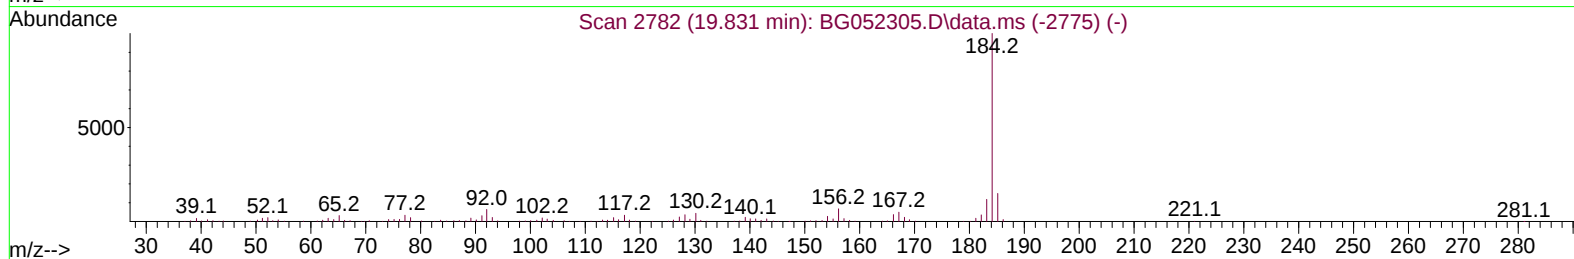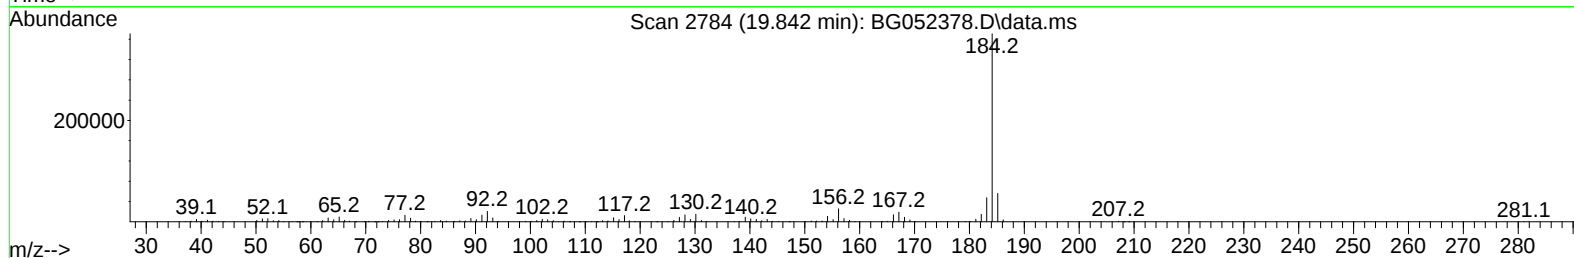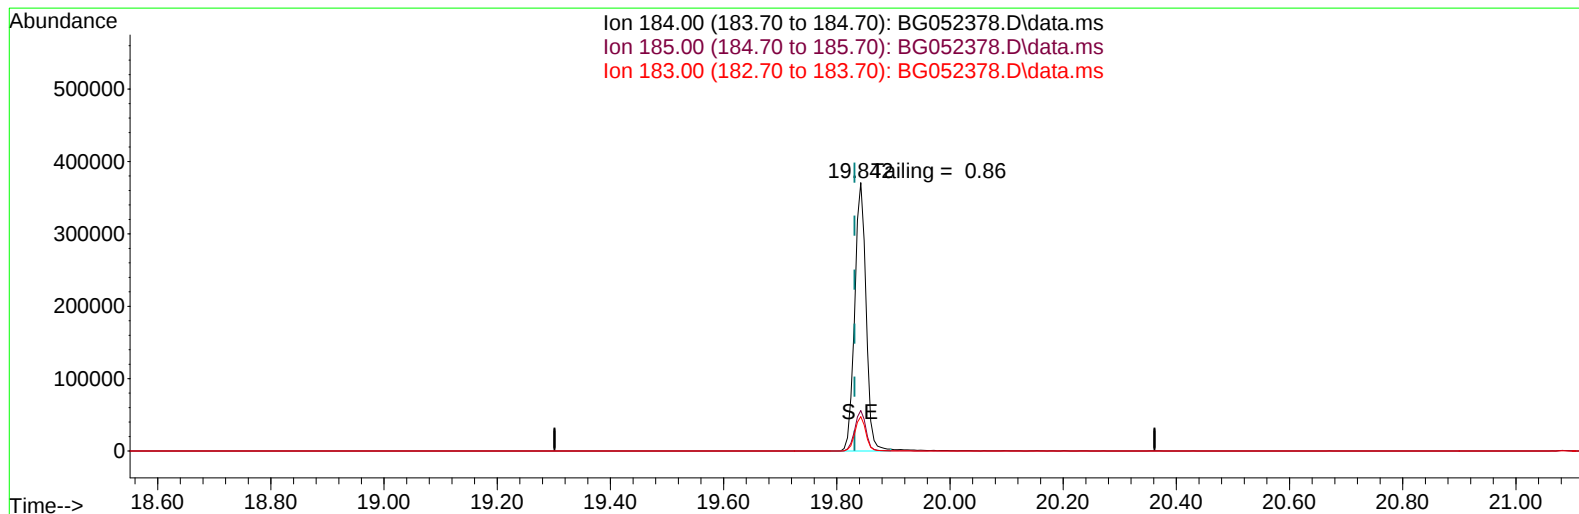

TIC: BG052378.D\data.ms

(77) Benzidine

19.842min (+ 0.011) 0.00 ng

response 523820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.11
183.00	12.20	12.81
0.00	0.00	0.00