
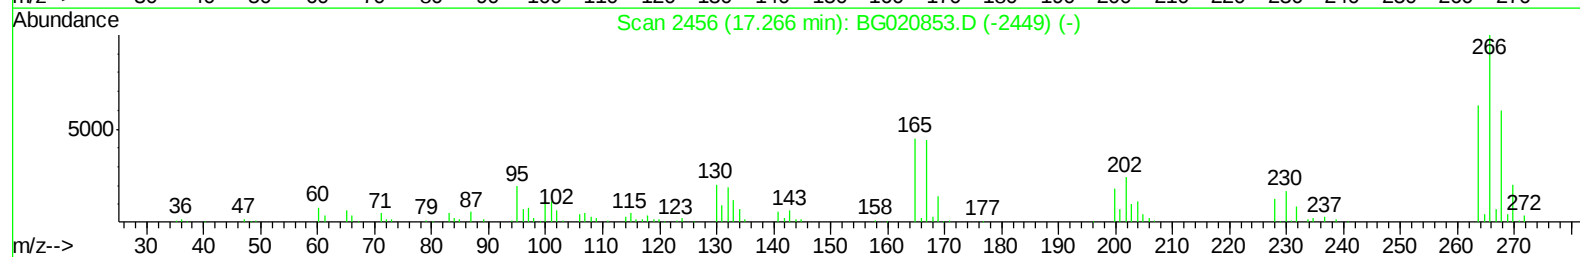
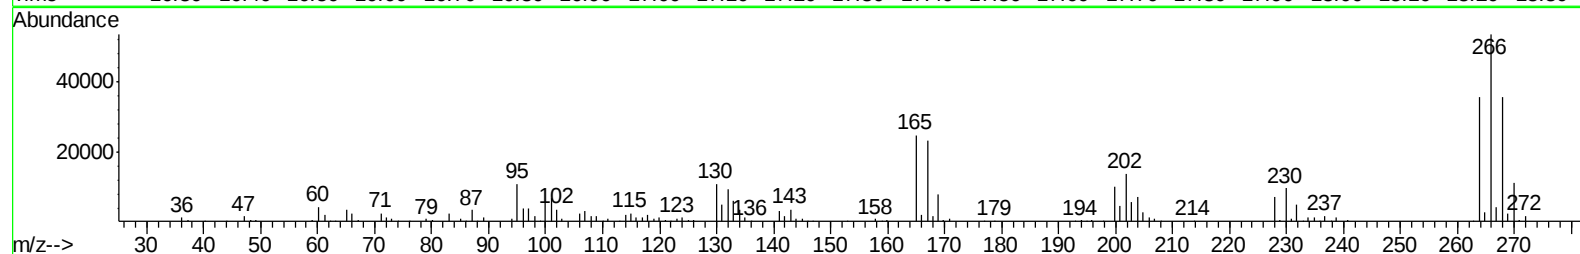


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021516\
Data File : BG020903.D
Acq On : 15 Feb 2016 9:51
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 06:43:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

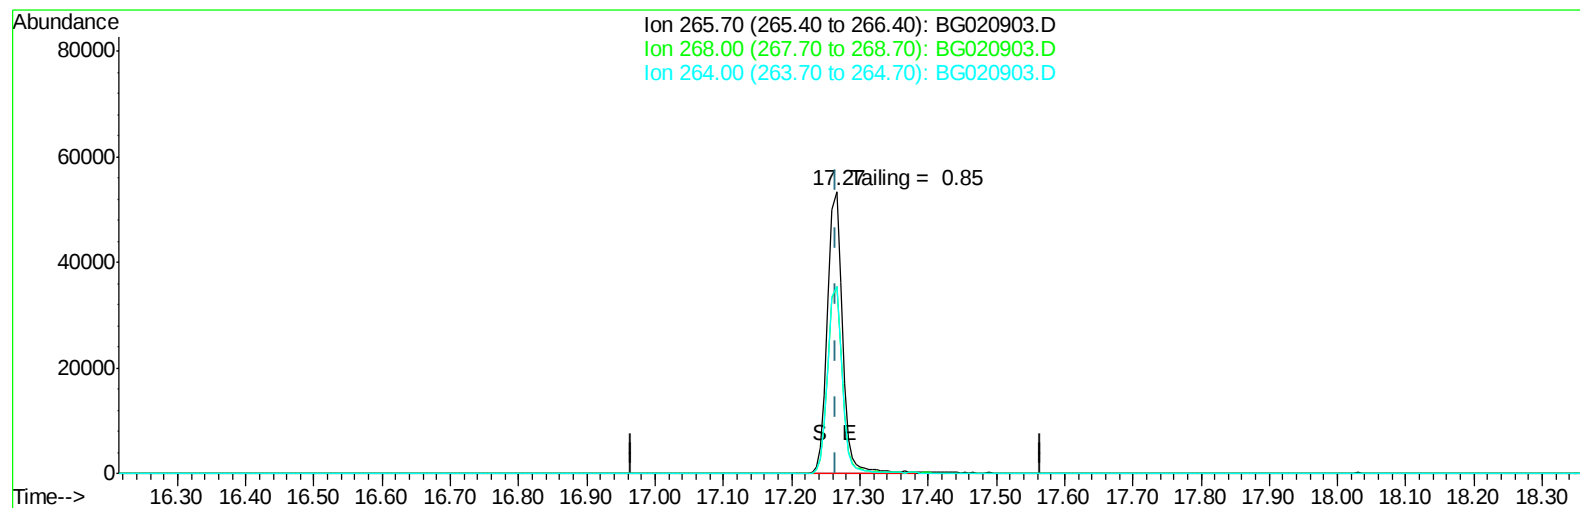

TIC: BG020903.D

(69) Pentachlorophenol (C)




17.266min (-0.000) 13956.43ng

response 80658

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	66.23
264.00	62.80	66.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG021516\
Data File : BG020903.D
Acq On : 15 Feb 2016 9:51
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 06:43:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

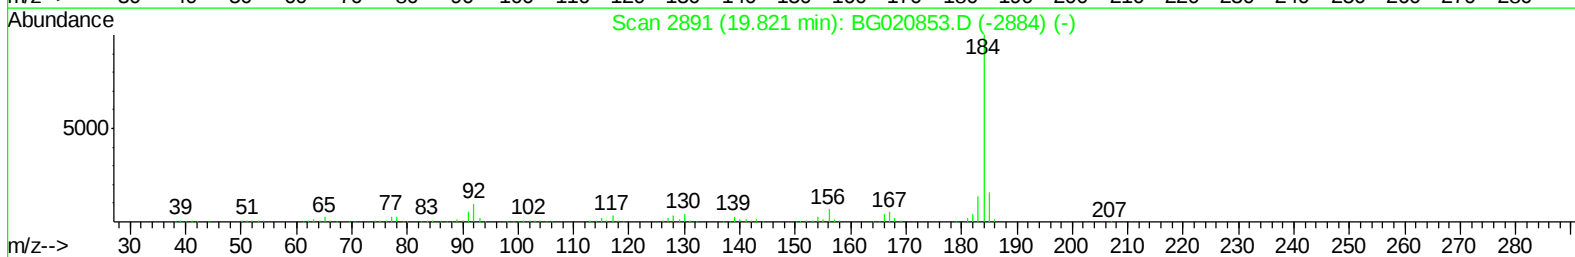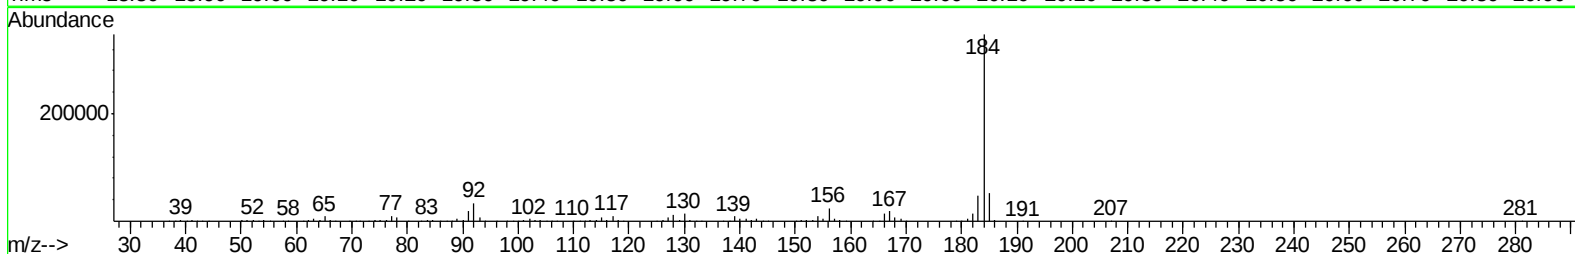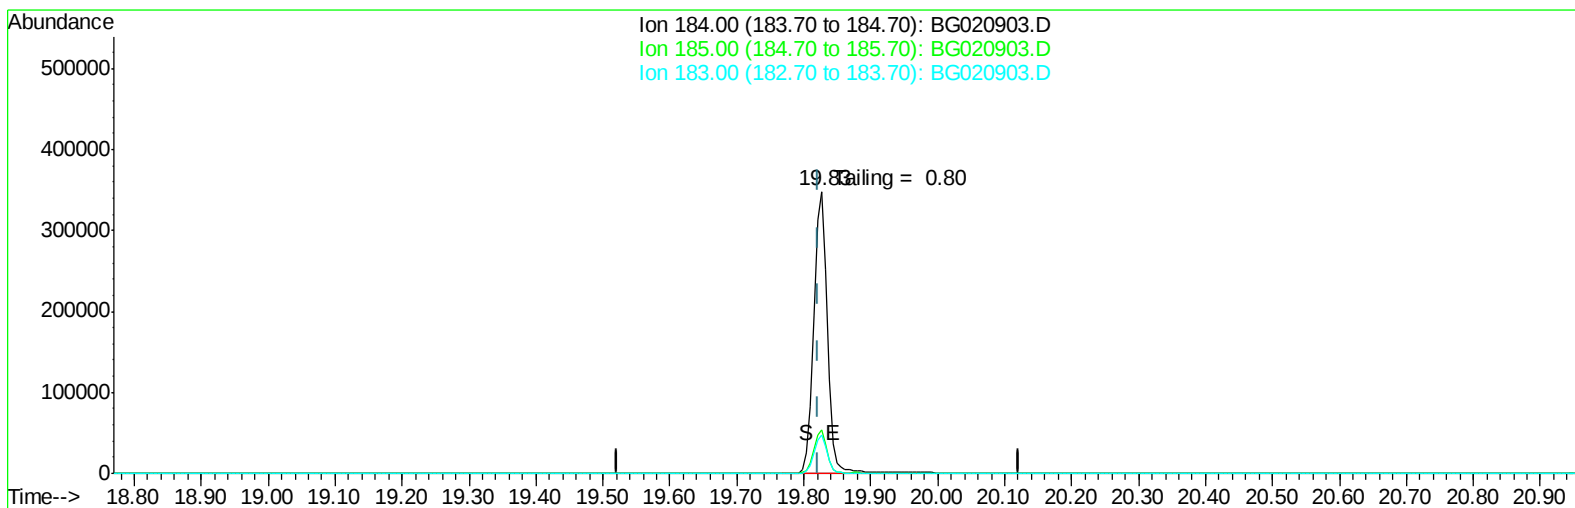

TIC: BG020903.D

(76) Benzidine

19.827min (+0.005) 0.00ng

response 503981

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.25
183.00	13.70	13.50
0.00	0.00	0.00