


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021516\
Data File : BG020903.D
Acq On : 15 Feb 2016 9:51
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 11 15:26:53 2016

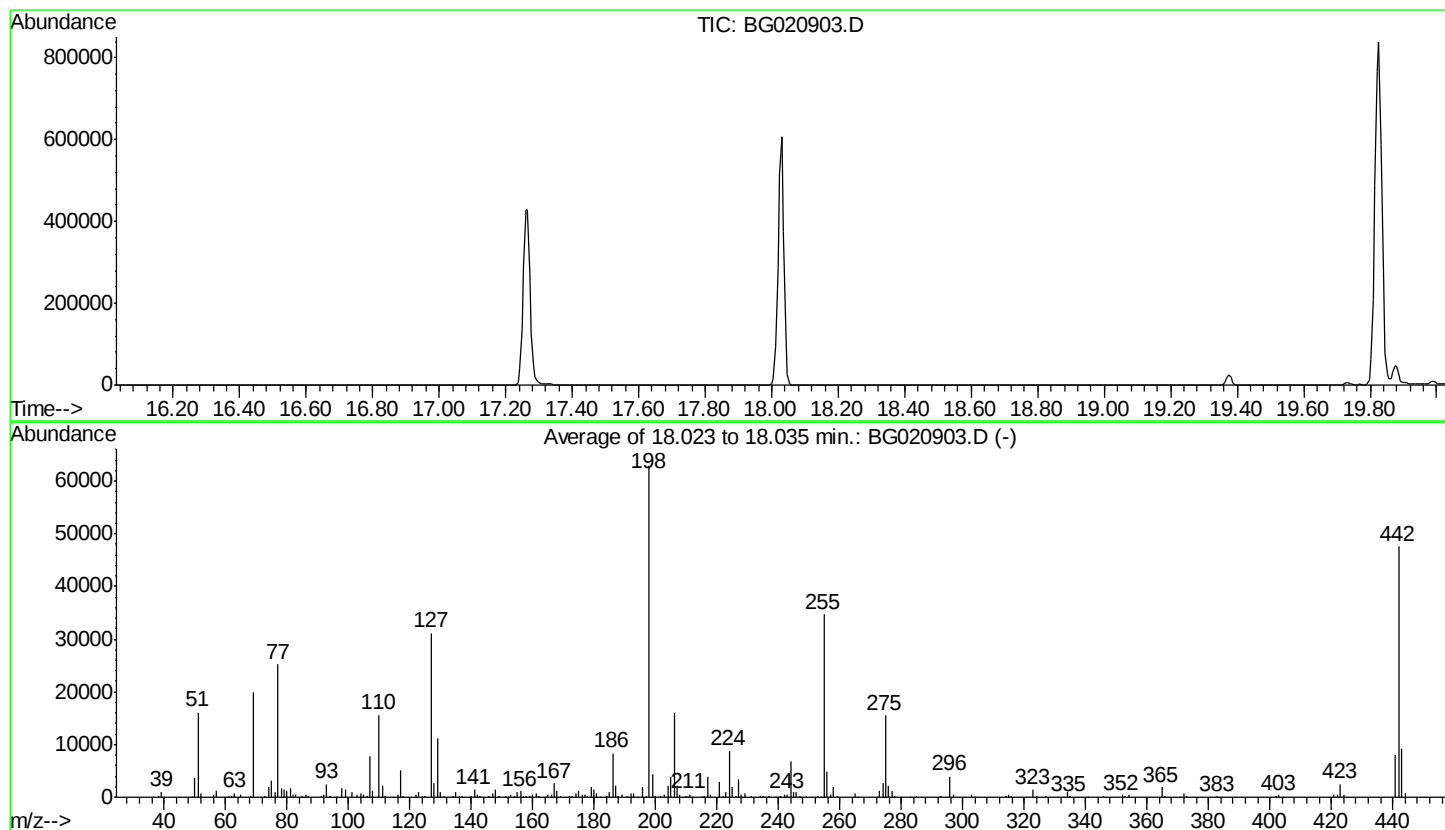

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	16076	PASS
68	69	0.00	2	1.0	203	PASS
69	198	0.00	100	31.5	19843	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	31136	PASS
197	198	0.00	2	0.2	141	PASS
198	198	100	100	100.0	62933	PASS
199	198	5	9	6.9	4354	PASS
275	198	10	60	24.6	15511	PASS
365	198	1	100	3.0	1860	PASS
441	442	0.01	24	16.8	7979	PASS
442	198	50	100	75.5	47522	PASS
443	442	15	24	19.6	9296	PASS