
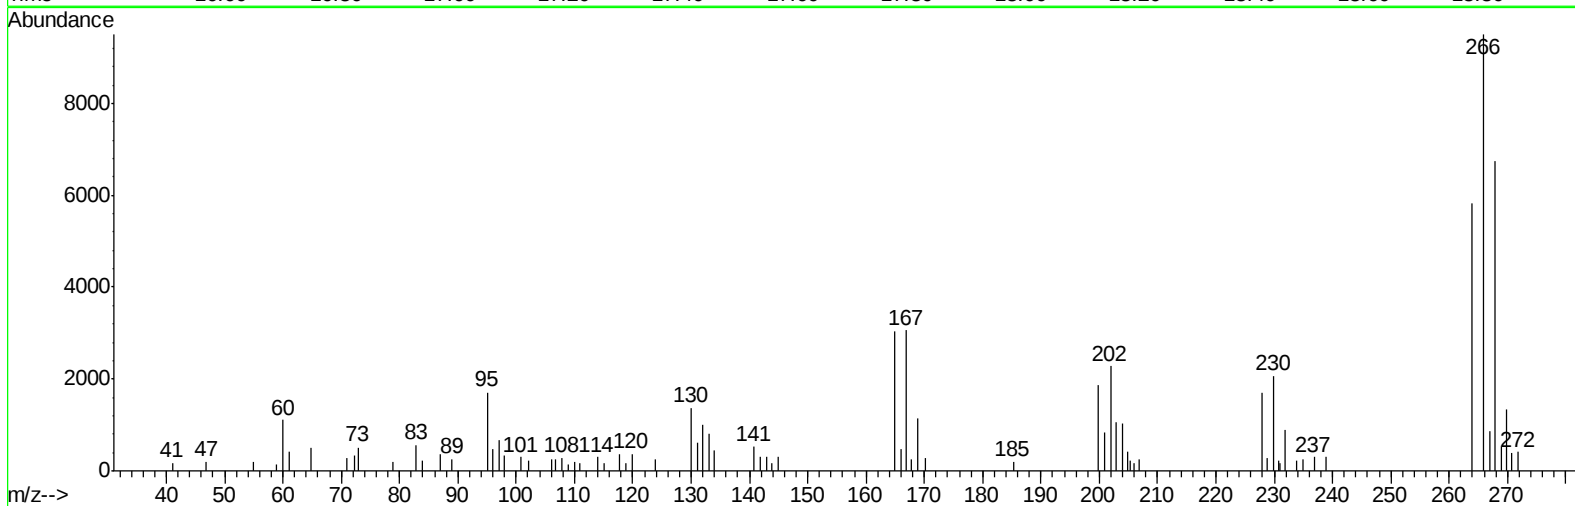


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021518\
Data File : BG032713.D
Acq On : 15 Feb 2018 14:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:38:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

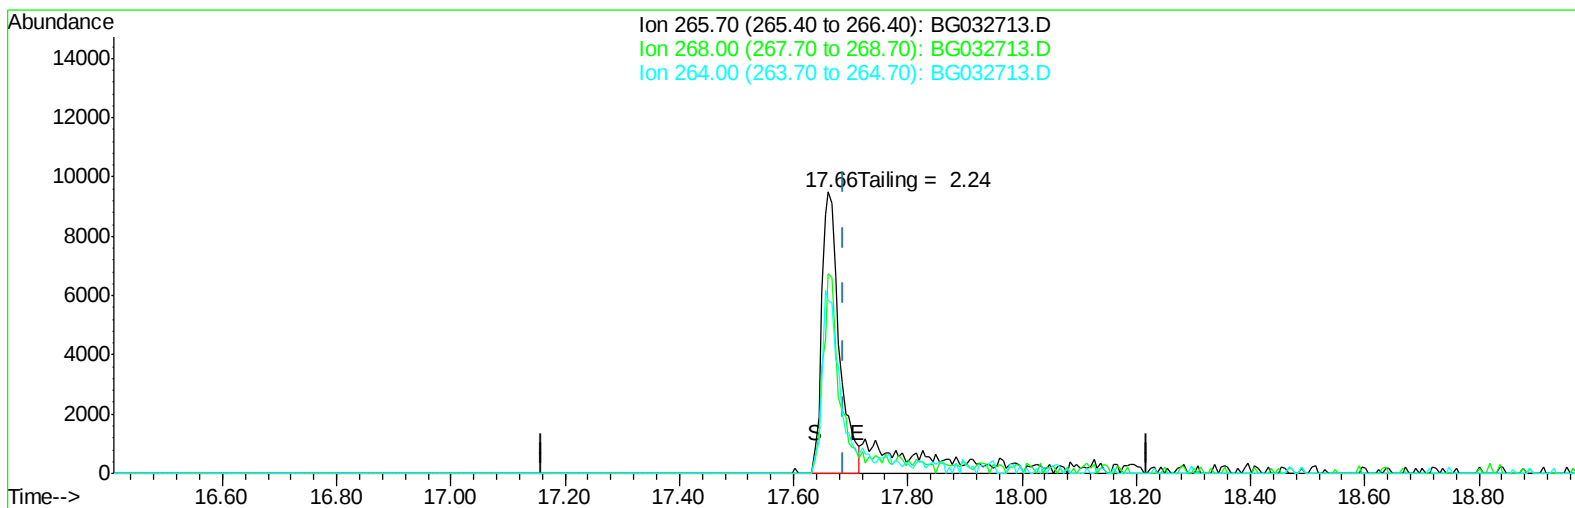

TIC: BG032713.D

(69) Pentachlorophenol (C)



17.661min (-0.028) 0.00ng

response 20255

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.91
264.00	62.00	61.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021518\
Data File : BG032713.D
Acq On : 15 Feb 2018 14:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:38:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

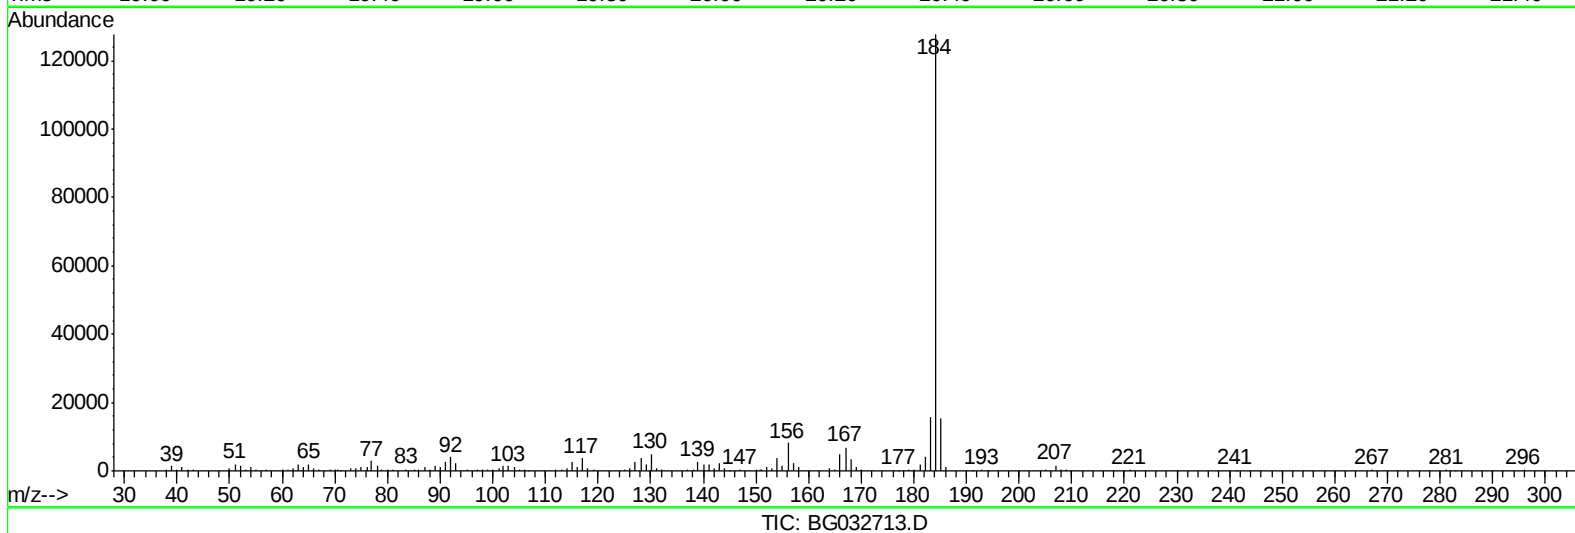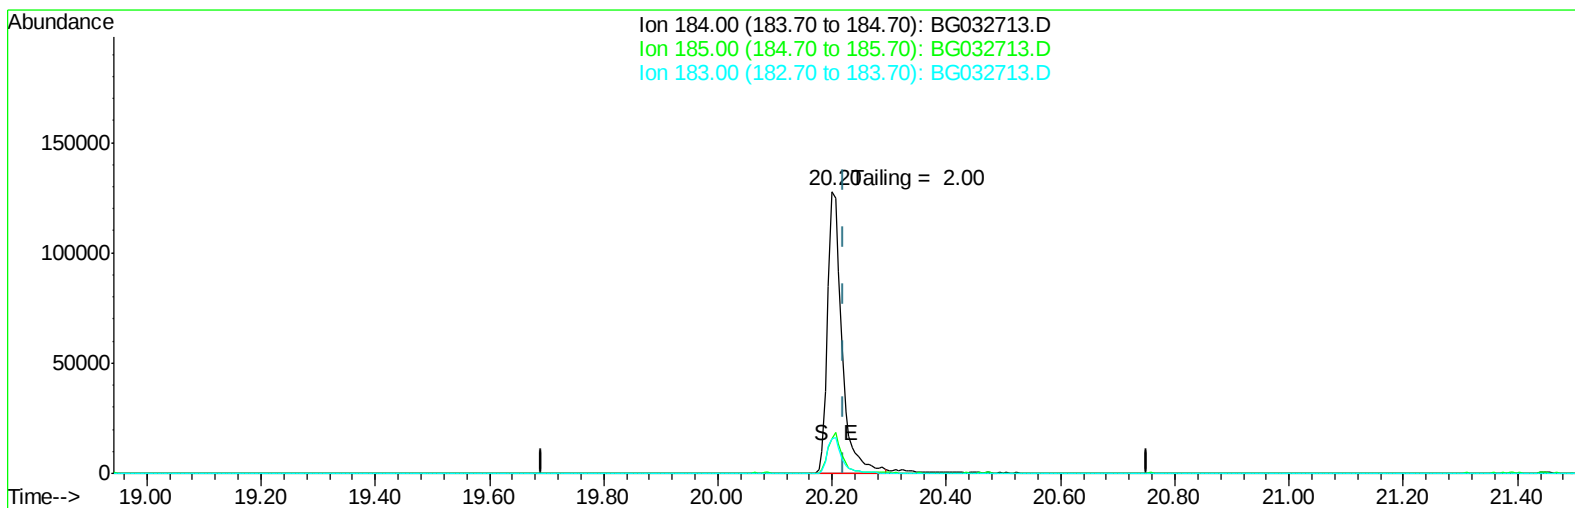

TIC: BG032713.D

(76) Benzidine

20.200min (-0.022) 170326.72ng

response 224603

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	12.07
183.00	13.30	12.44
0.00	0.00	0.00