
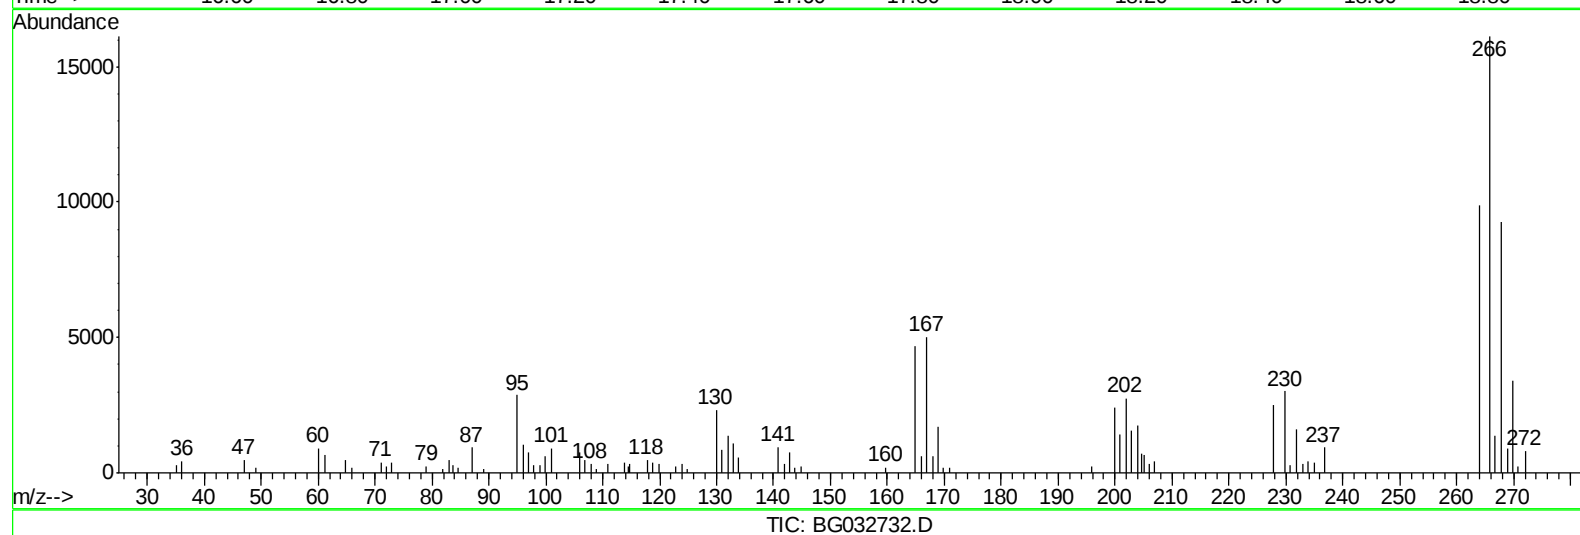


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021518\
Data File : BG032732.D
Acq On : 16 Feb 2018 2:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:41:00 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

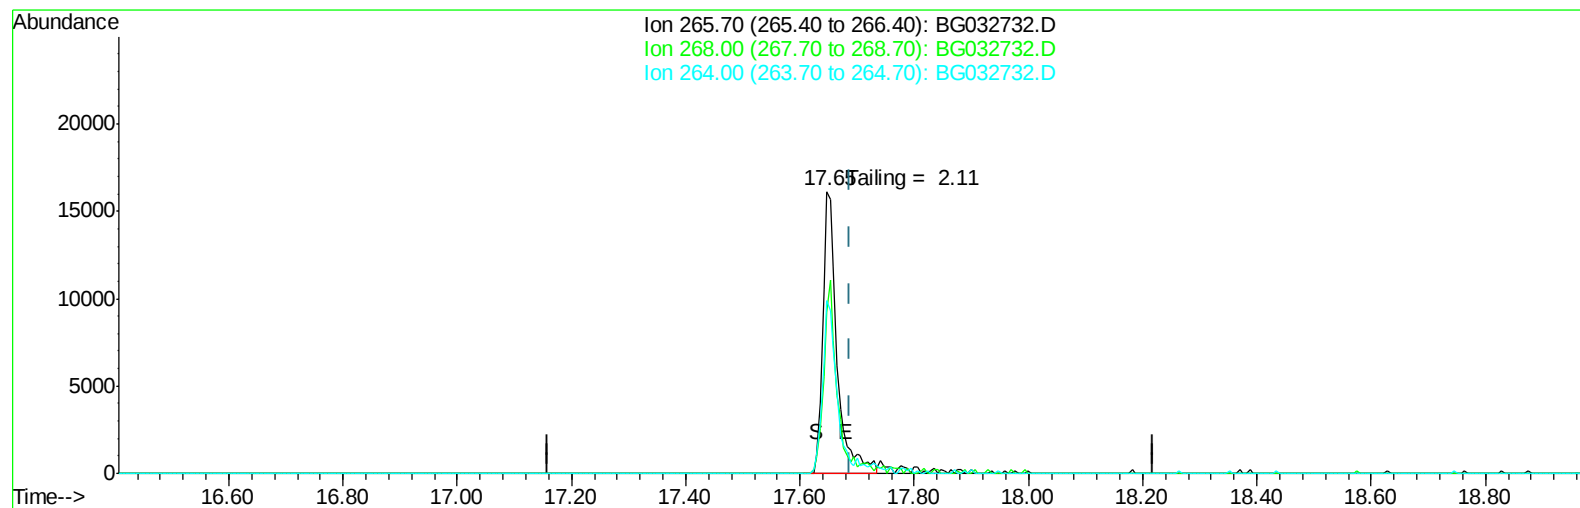

(69) Pentachlorophenol (C)



17.647min (-0.042) 48358.51ng

response 28214

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.39
264.00	62.00	61.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021518\
Data File : BG032732.D
Acq On : 16 Feb 2018 2:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:41:00 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 18:08:01 2018
Response via : Initial Calibration

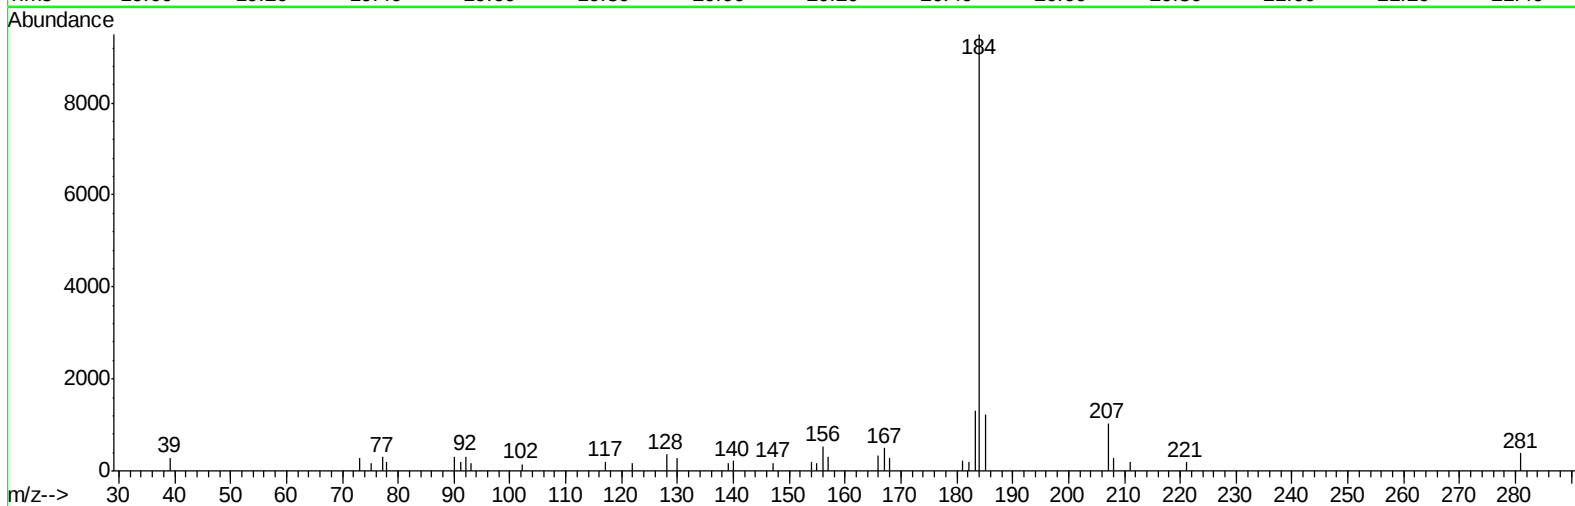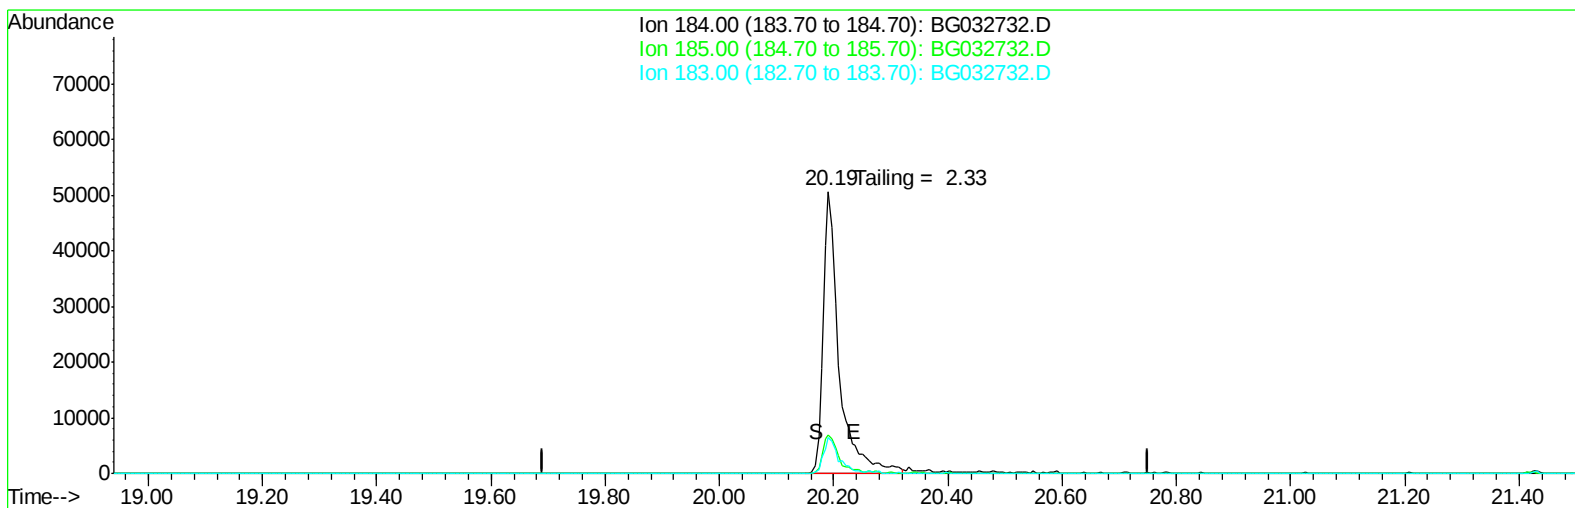

TIC: BG032732.D

(76) Benzidine

20.221min (-20.221) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00