


Data Path : Z:\HPCHEM1\BNA G\Data\BG021518\
 Data File : BG032713.D
 Acq On : 15 Feb 2018 14:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 12 18:08:01 2018

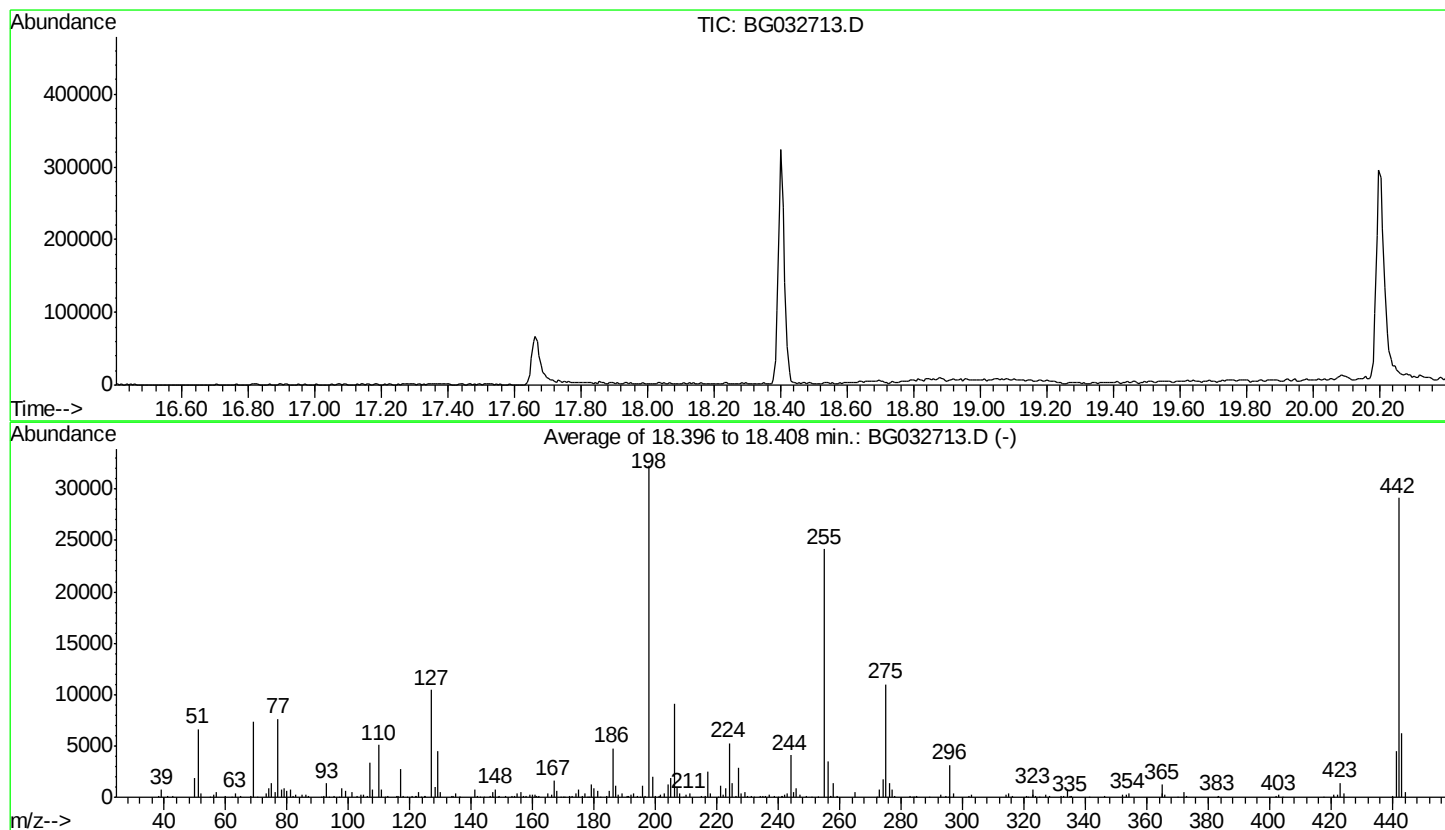

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	6670	PASS
68	69	0.00	2	1.5	112	PASS
69	198	0.00	100	22.8	7353	PASS
70	69	0.00	2	0.9	66	PASS
127	198	10	80	32.4	10454	PASS
197	198	0.00	2	0.3	96	PASS
198	198	100	100	100.0	32282	PASS
199	198	5	9	6.0	1953	PASS
275	198	10	60	34.2	11025	PASS
365	198	1	100	3.8	1224	PASS
441	442	0.01	24	15.6	4535	PASS
442	198	50	100	90.2	29114	PASS
443	442	15	24	21.3	6188	PASS