

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052389.D
 Acq On : 15 Feb 2022 10:41
 Operator : CG/JU
 Sample : PB142594BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	6	10	17	rVB2	8644	12434	1.24%	0.136%
2	3.975	79	83	96	rBV	95518	161390	16.05%	1.762%
3	4.081	100	101	104	rVV3	1526	1365	0.14%	0.015%
4	4.574	182	185	190	rBV3	813	1534	0.15%	0.017%
5	7.370	655	661	669	rBV	120968	205285	20.41%	2.241%
6	7.535	682	689	698	rVB	89501	153407	15.25%	1.675%
7	7.752	719	726	735	rVB	110027	190656	18.96%	2.082%
8	8.228	800	807	816	rBV	92356	147425	14.66%	1.610%
9	8.933	920	927	935	rBV	150811	251878	25.04%	2.750%
10	9.397	998	1006	1016	rVV	119543	212174	21.10%	2.317%
11	10.131	1123	1131	1142	rBV	103676	182658	18.16%	1.994%
12	10.678	1218	1224	1236	rBV	136599	253284	25.18%	2.765%
13	11.065	1283	1290	1299	rVB	123854	223207	22.19%	2.437%
14	11.189	1304	1311	1322	rBV	145721	265236	26.37%	2.896%
15	12.646	1554	1559	1564	rVB2	2449	3901	0.39%	0.043%
16	14.261	1827	1834	1842	rBV	307154	456107	45.35%	4.980%
17	14.566	1879	1886	1894	rVB	340123	536926	53.39%	5.862%
18	14.872	1931	1938	1945	rBV	214833	342129	34.02%	3.736%
19	15.060	1964	1970	1986	rBV	105259	205632	20.45%	2.245%
20	15.271	2003	2006	2012	rVB4	898	2013	0.20%	0.022%
21	15.859	2100	2106	2114	rBV	439897	676173	67.23%	7.383%
22	15.970	2120	2125	2137	rBV	124000	185842	18.48%	2.029%
23	16.100	2143	2147	2153	rBV2	1904	2284	0.23%	0.025%
24	17.404	2367	2369	2373	rVB2	1380	1433	0.14%	0.016%
25	17.615	2399	2405	2413	rVB	304433	467890	46.52%	5.109%
26	17.715	2416	2422	2432	rVV	528227	798107	79.36%	8.714%
27	19.566	2733	2737	2740	rBV2	8061	10396	1.03%	0.114%
28	19.636	2744	2749	2753	rBV	6615	9299	0.92%	0.102%
29	19.742	2765	2767	2770	rVB3	1565	1670	0.17%	0.018%
30	19.994	2802	2810	2824	rBV	690276	1005716	100.00%	10.981%
31	20.176	2839	2841	2846	rVB2	1122	1614	0.16%	0.018%
32	20.364	2870	2873	2876	rVB3	1569	2054	0.20%	0.022%
33	20.946	2969	2972	2973	rBV2	2176	1913	0.19%	0.021%
34	21.052	2987	2990	2991	rBV2	1953	2313	0.23%	0.025%
35	21.158	3006	3008	3010	rBV2	1331	1328	0.13%	0.014%
36	21.228	3017	3020	3022	rBV4	2041	2860	0.28%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052389.D
 Acq On : 15 Feb 2022 10:41
 Operator : CG/JU
 Sample : PB142594BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.387	3045	3047	3051	rBV4	1933	2895	0.29%	0.032%
38	21.563	3075	3077	3079	rBV2	2091	2128	0.21%	0.023%
39	21.933	3133	3140	3151	rVB	309165	538943	53.59%	5.884%
40	22.139	3173	3175	3178	rBV3	1610	1347	0.13%	0.015%
41	22.415	3221	3222	3224	rVB2	2447	1354	0.13%	0.015%
42	22.661	3262	3264	3266	rBV2	1776	1748	0.17%	0.019%
43	22.749	3277	3279	3285	rBV4	2996	4445	0.44%	0.049%
44	23.225	3358	3360	3361	rBV2	1597	1350	0.13%	0.015%
45	23.384	3385	3387	3389	rBV3	1672	1960	0.19%	0.021%
46	23.490	3403	3405	3406	rBV2	2112	2123	0.21%	0.023%
47	23.578	3417	3420	3423	rBV4	1583	1733	0.17%	0.019%
48	23.777	3452	3454	3456	rBV2	1992	1310	0.13%	0.014%
49	24.312	3542	3545	3547	rBV4	1997	2661	0.26%	0.029%
50	24.330	3547	3548	3550	rVB2	3143	1788	0.18%	0.020%
51	24.377	3550	3556	3557	rBV6	6145	10231	1.02%	0.112%
52	24.471	3571	3572	3574	rBV2	3290	2167	0.22%	0.024%
53	24.905	3644	3646	3649	rBV3	1872	1816	0.18%	0.020%
54	25.070	3672	3674	3675	rVV2	2332	1509	0.15%	0.016%
55	25.158	3678	3689	3701	rVV	322423	943415	93.81%	10.301%
56	25.399	3719	3730	3743	rVB2	181378	531341	52.83%	5.801%
57	25.693	3777	3780	3783	rBV2	2442	3101	0.31%	0.034%
58	25.910	3816	3817	3819	rBV2	2097	1723	0.17%	0.019%
59	26.121	3852	3853	3855	rBV2	2583	1317	0.13%	0.014%
60	26.292	3880	3882	3885	rBV4	1852	2489	0.25%	0.027%
61	26.321	3885	3887	3889	rVB3	1961	1449	0.14%	0.016%
62	26.644	3939	3942	3953	rVB10	7368	21292	2.12%	0.232%
63	26.997	3999	4002	4003	rBV3	2491	2308	0.23%	0.025%
64	27.026	4006	4007	4010	rBV2	2285	2512	0.25%	0.027%
65	27.120	4021	4023	4025	rBV2	1952	1739	0.17%	0.019%
66	27.484	4084	4085	4088	rBV3	2292	1490	0.15%	0.016%
67	27.690	4119	4120	4122	rVB2	2997	1982	0.20%	0.022%
68	27.719	4122	4125	4128	rBV4	3612	5413	0.54%	0.059%
69	27.966	4165	4167	4168	rVB2	2960	1599	0.16%	0.017%
70	27.989	4168	4171	4173	rBV4	2129	2181	0.22%	0.024%
71	28.113	4189	4192	4193	rBV2	4124	3893	0.39%	0.043%
72	28.289	4220	4222	4224	rVV2	2158	1401	0.14%	0.015%
73	28.418	4241	4244	4246	rBV3	2212	2762	0.27%	0.030%
74	28.594	4272	4274	4276	rVB3	3143	2802	0.28%	0.031%
75	28.618	4276	4278	4280	rBV3	2190	2485	0.25%	0.027%
76	28.953	4333	4335	4337	rVB3	2212	1723	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052389.D
 Acq On : 15 Feb 2022 10:41
 Operator : CG/JU
 Sample : PB142594BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	29.294	4391	4393	4395	rBV3	1726	1573	0.16%	0.017%
78	29.529	4432	4433	4436	rVB3	2883	1482	0.15%	0.016%
79	29.628	4449	4450	4452	rVB	2534	1650	0.16%	0.018%
80	29.705	4461	4463	4465	rBV3	1973	1580	0.16%	0.017%
81	29.740	4468	4469	4472	rBV3	2806	2713	0.27%	0.030%
82	29.805	4478	4480	4484	rBV3	2362	2697	0.27%	0.029%
83	29.881	4489	4493	4494	rBV4	2921	3649	0.36%	0.040%
84	29.928	4499	4501	4508	rVB5	4267	8889	0.88%	0.097%
85	30.134	4534	4536	4540	rVB5	2446	2203	0.22%	0.024%
86	30.169	4540	4542	4543	rBV2	2338	1386	0.14%	0.015%
87	30.286	4560	4562	4565	rBV4	1706	1738	0.17%	0.019%
88	30.903	4663	4667	4670	rBV5	2692	3601	0.36%	0.039%
89	30.956	4675	4676	4678	rBV2	1934	1449	0.14%	0.016%
90	31.027	4686	4688	4689	rBV	1712	1294	0.13%	0.014%
91	31.044	4689	4691	4692	rVV2	3153	1983	0.20%	0.022%
92	31.085	4696	4698	4700	rVB3	2213	2033	0.20%	0.022%
93	31.261	4726	4728	4729	rBV2	2370	1955	0.19%	0.021%
94	31.355	4742	4744	4747	rBV3	2001	2248	0.22%	0.025%
95	31.420	4753	4755	4758	rBV4	2517	2817	0.28%	0.031%
96	31.449	4758	4760	4763	rVV4	1815	2010	0.20%	0.022%
97	31.508	4768	4770	4771	rBV2	1790	1384	0.14%	0.015%
98	31.538	4773	4775	4779	rVV5	2101	2350	0.23%	0.026%
99	31.655	4793	4795	4796	rBV	2500	1394	0.14%	0.015%
100	32.066	4863	4865	4868	rBV4	3657	3295	0.33%	0.036%




Sum of corrected areas: 9158831

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052389.D
Acq On : 15 Feb 2022 10:41
Operator : CG/JU
Sample : PB142594BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

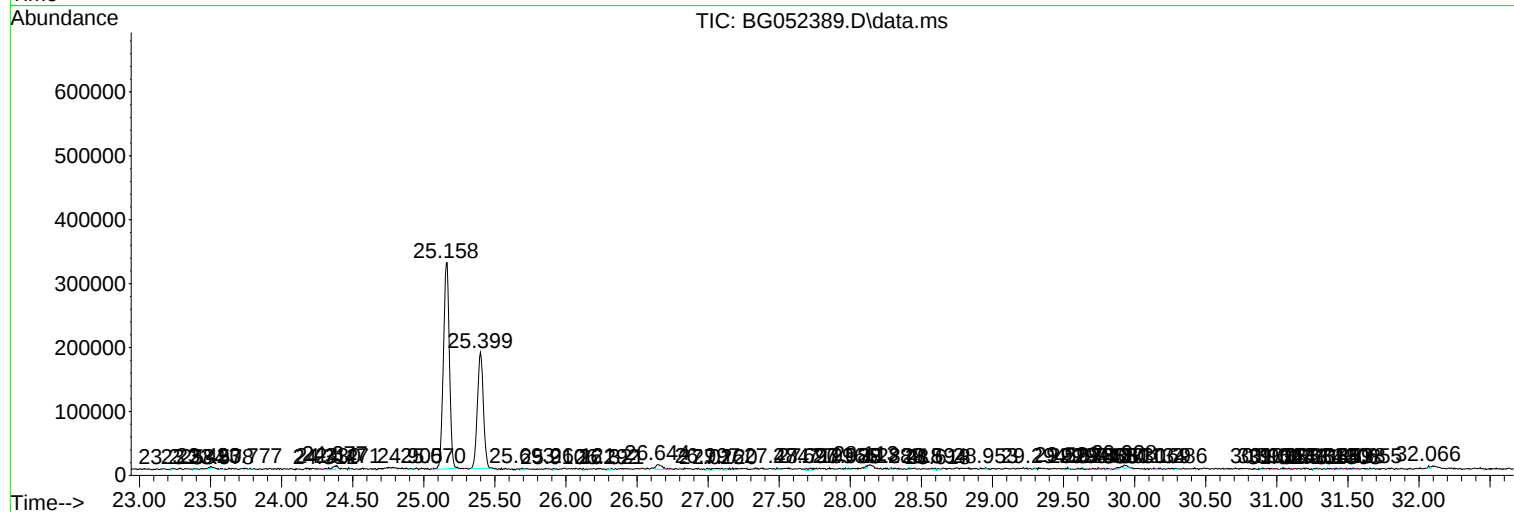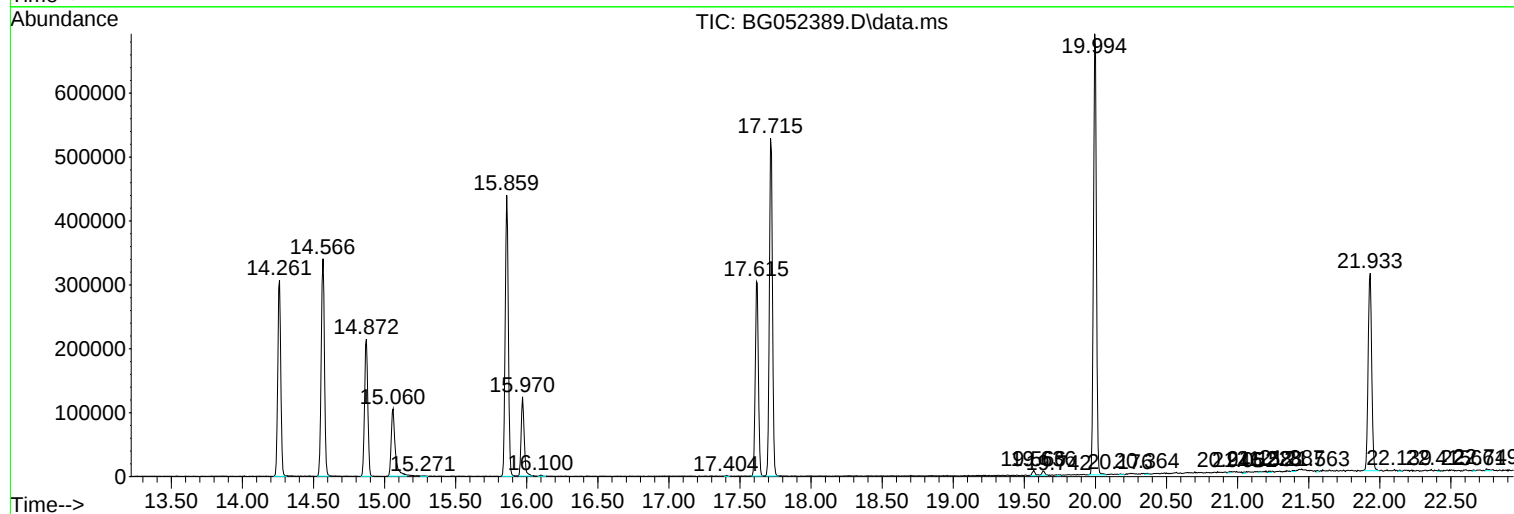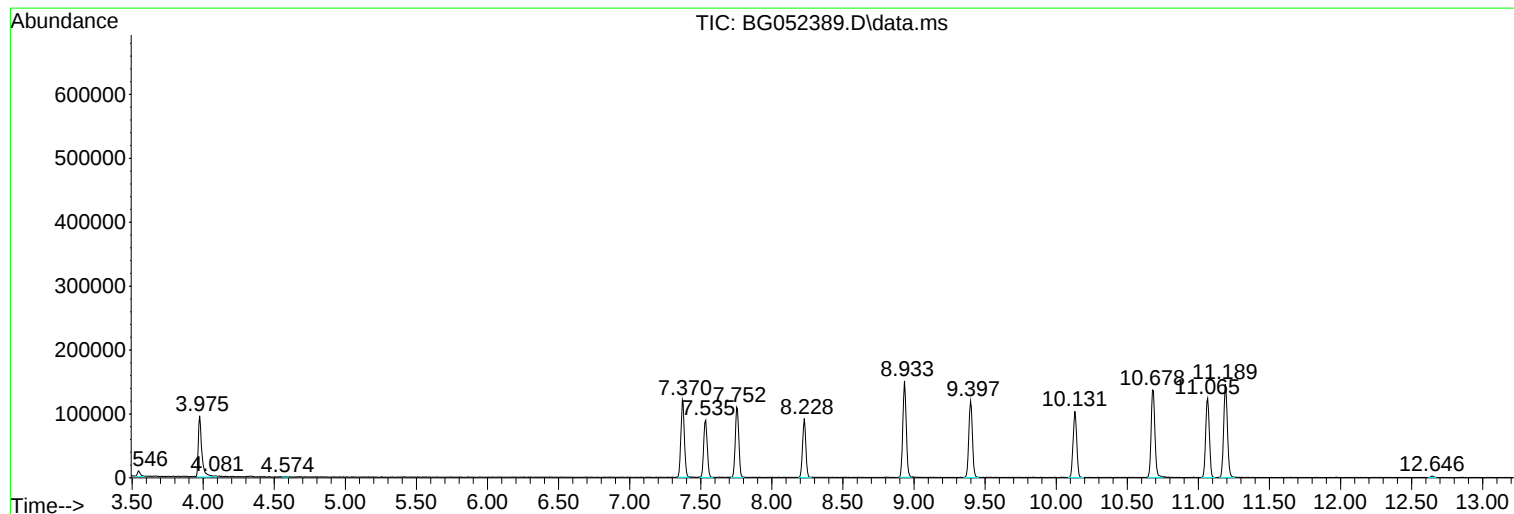

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052389.D
Acq On : 15 Feb 2022 10:41
Operator : CG/JU
Sample : PB142594BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052389.D
Acq On : 15 Feb 2022 10:41
Operator : CG/JU
Sample : PB142594BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
